CONTRACT NO. 93-300 FINAL REPORT MAY 1994



Measurement of Atmospheric Nitric Acid at Azusa by Tunable Diode Laser Absorption Spectrometry



CALIFORNIA ENVIRONMENTAL PROTECTION AGENCY



AIR RESOURCES BOARD Research Division

		,		

# Measurement of Atmospheric Nitric Acid at Azusa by Tunable Diode Laser Absorption Spectrometry

# Final Report

Contract No. 93-300

## Prepared for:

California Air Resources Board Research Division 2020 L Street Sacramento, California 95814

# Prepared by:

Gervase I. Mackay, Ph.D.

UNISEARCH ASSOCIATES INC. 222 Snidercroft Rd Concord, Ontario L4K 1B5 CANADA

	,		

Final Report to the

## STATE OF CALIFORNIA AIR RESOURCES BOARD

in

completion of research under agreement number 93-300

## **DISCLAIMER**

The statements and conclusions in this report are those of Unisearch Associates Inc. and not necessarily those of the Contractor. The mention of commercial products, their source or their use in connection with material reported herein is not to be construed as actual or implied endorsement of such products.

#### **ACKNOWLEDGMENTS**

This work was funded by the State of California Air Resources Board, agreement number 93-300. We thank Dr. Lowell Ashbaugh for making the arrangements with the South Coast Air Quality Management District (SCAQMD) for the use of the Azusa AQMD monitoring site. We are most thankful to Dr. Clint Taylor of ARB Sacramento for analyzing the permeation tube bubblers and providing us with an accurate determination of the HNO<sub>3</sub> permeation rate.

We also gratefully acknowledge the SCAQMD for providing the site and thank the station Technologist, Mr. Sumner Wilson, for his assistance during the study.

	•		
		,	

### **EXECUTIVE SUMMARY**

HNO<sub>3</sub> plays an important role in the photochemistry of urban and rural air and its accurate measurement provides a sensitive test for current acid deposition models. Measurements of nitric acid (HNO<sub>3</sub>) by denuder tube technology are made on a routine basis in the Southern California acid deposition network. Recently, the HNO<sub>3</sub> results from a number of these stations have shown variability inconsistent with the expected behavior. It was thought to be prudent, therefore, to compare the measurements with a reference standard air monitoring technique at one of these sites which might help to identify the source of the variability.

Tunable diode laser absorption spectroscopy (TDLAS) offers a number of advantages for making this measurement. Its high spectral resolution provides an unequivocal identification of the measured gaseous species free from interferences of other atmospheric constituents. This specificity makes it an ideal instrument to use as a standard against which other, less definitive methods, can be compared. In addition the TDLAS has high sensitivity and rapid response time so that it can provide real time measurements with detection limits much better than those required for ambient concentrations of the majority of trace constituents under most atmospheric conditions.

The Unisearch model TAMS-150 TDLAS was employed for the measurement of HNO<sub>3</sub> and had detection limits of better than 0.2 ppbv.

Measurements of HNO<sub>3</sub> by the TDLAS were made during the period 12:00, September 30, 1993 through 24:00, October 30, 1993 inclusive. Data was obtained over 1 minute averaging periods. The results have also been reduced to 1 hour average values and Daytime average value (10:00 - 18:00) for comparison with measurements made by the ARB denuder samplers. Data coverage was better than 98%.

The diurnal behavior of HNO<sub>3</sub> was quite regular. The maximum concentrations generally occurred between 14:00 and 16:00 each day. The HNO<sub>3</sub> daily maximum varied between 3 ppbv (during wet weather) and 30 ppbv (hot dry weather) with the median value of about 15 ppbv for the entire period. The averages calculated for the period 10:00 -- 18:00 (the denuder sampling period) were on average twice the nighttime (18:00 -- 10:00) average and represented ~75% of the total daily HNO<sub>3</sub> burden. This indicates that, on most occasions, the denuders should capture a major fraction of the HNO<sub>3</sub> produced during a 24 hour period.

There was no evidence for any large particle nitrate (>2  $\mu$ m) dissociation from the particulate matter collected on the inlet filter contributing to the IINO<sub>3</sub> signal measured by the TDLAS. While it could not be completely ruled out, dissociation of small nitrate particles (<2  $\mu$ m) (which passed through the filter) in the White cell was not obvious and the results indicate that it could contribute at most 10% of the measured signal at any time.

•			
•			

TABLE OF	CONTENTSPAG	E
DISCLAIM	ER	, i
ACKNOWL	LEDGMENTS	ii
1. INTROD	UCTION	1
2. EXPERIN	MENTAL	2
2.1	PRINCIPLE OF THE TDLAS SYSTEM	2
2.2	SAMPLING AND CALIBRATION PROCEDURES.	2
Į.	FIGURE 1: RESPONSE TIME OF THE TDLAS TO A 6.9 PPBV SPIKE OF HNO <sub>3</sub> ADDED INTO THE AMBIENT PRESSURE SIDE OF THE SAMPLING LINE ~1 M UPSTREAM OF THE WHITE CELL. EFFICIENCY OF THE BACKGROUND SCRUBBER IS ALSO DEMONSTRATED.	3
( !	FIGURE 2: .DIURNAL VARIATION IN AMBIENT HNO <sub>3</sub> AND THE MEASURED BACKGROUND SIGNAL OBTAINED BY PASSING AMBIENT AIR THROUGH A 1 µM PORE SIZE NYLON FILTER ON OCTOBER 22, 1993. BACKGROUND MEASUREMENTS MADE EVERY 15 MINUTES WERE COMBINED TO PROVIDE HOURLY AVERAGE VALUES.	5
2.3	HNO <sub>3</sub> REFERENCE STANDARD CALIBRATION PROCEDURES.	6
П	TABLE 1: PERMEATION RATES FOR THE UNISEARCH HNO <sub>3</sub> PERMEATION DEVICE DETERMINED BY ITTRATION AGAINST STANDARD NAOH PREPARED PRIOR TO THE FIELD STUDY USING LAB DISTILLED WATER (1, 2, 3 AND 10) AND LOCAL STORE DE IONIZED WATER (3 9)	7
r (	TABLE 2: PERMEATION RATES FOR THE UNISEARCH HNO <sub>3</sub> PERMEATION DEVICE DETERMINED BY ION CHROMATOGRAPHY FROM SAMPLES OBTAINED DURING THE FIELD STUDY.	8
1 J	TABLE 3: PERMEATION RATES FOR THE UNISEARCH HNO <sub>3</sub> PERMEATION DEVICE DETERMINED AT THE UNISEARCH LABORATORY SUBSEQUENT TO THE FIELD STUDY	8
3. AMBIEN	T AIR MEASUREMENTS HNO3	9
3.11	EXPERIMENTAL CONFIGURATION	9
3.2 [	MEASUREMENT PROCEDURE	9
4. RESULTS	S AND DISCUSSION10	0
C	FIGURE 3: .DIURNAL VARIATION IN THE ONE HOUR AVERAGE AMBIENT HNO <sub>3</sub> MEASURED BY THE TDLAS ON OCTOBER 25, 1993. THE LOWER TRACE IS THE CALCULATED HOURLY AVERAGE CONFIDENCE LIMIT WHICH IS COMPARABLE TO THE MINIMUM DETECTION LIMIT FOR THAT PERIOD	
L T	FIGURE 4: DIURNAL VARIATION IN THE ONE HOUR AVERAGE AMBIENT HNO <sub>3</sub> MEASURED BY THE TDLAS DURING THE PERIOD 12:00, SEPTEMBER 30, 1993, THROUGH 24:00, OCTOBER 30, 1993. THE LOWER TRACE IS THE CALCULATED HOURLY AVERAGE CONFIDENCE LIMIT WHICH IS COMPARABLE TO THE MINIMUM DETECTION LIMIT FOR THAT PERIOD.	1
() A	FIGURE 5: DAILY AVERAGE HNO <sub>3</sub> MIXING RATIOS MEASURED BY THE TDLAS DURING THE PERIOD 00:00 OCTOBER 1, 1993, THROUGH 24:00, OCTOBER 30, 1993. THE LOWER TRACE IS THE CALCULATED DAILY AVERAGE CONFIDENCE LIMIT WHICH IS COMPARABLE TO THE MINIMUM DETECTION LIMIT FOR THAT PERIOD	
n T	FIGURE 6: DAYTIME (10:00 18:00) AVERAGE HNO <sub>3</sub> MIXING RATIOS MEASURED BY THE TDLAS OURING THE PERIOD 00:00, OCTOBER 1, 1993, THROUGH 24:00, OCTOBER 30, 1993. THE LOWER TRACE IS THE CALCULATED DAYTIME AVERAGE CONFIDENCE LIMIT WHICH IS COMPARABLE TO THE MINIMUM DETECTION LIMIT FOR THAT PERIOD	

TABLE OF CONTENTS CONTINUEDPAGE
TABLE 4: DAILY AVERAGE HNO <sub>3</sub> MIXING RATIO MEASURED BY THE TDLAS DURING THE LA ACID PRECIPITATION INTERCOMPARISON STUDY OCTOBER 1 30, 1993 AT THE AZUSA SCAQMD SITE 14
TABLE 5: DAYTIME (10:00 18:00) AVERAGE HNO <sub>3</sub> MIXING RATIO MEASURED BY THE TDLAS DURING THE LA ACID PRECIPITATION INTERCOMPARISON STUDY OCTOBER 1 30, 1993 AT THE AZUSA SCAQMD SITE
TABLE 6: AVERAGE HNO <sub>3</sub> MIXING RATIO FOR THE NON-DAYTIME AVERAGING PERIOD (18:00 10:00) MEASURED BY THE TDLAS DURING THE LA ACID PRECIPITATION INTERCOMPARISON STUDY OCTOBER 1 30, 1993 AT THE AZUSA SCAQMD SITE
4. CONCLUSIONS 17
5. REFERENCES 18
APPENDIX A

#### 1. INTRODUCTION

Nitric acid is a major final product for "odd nitrogen" in the atmosphere and its measurement is important in evaluating nitrogen photochemistry. It is also a major component in acid deposition. It is particularly important in the South Coast Air Basin [1] where the ratios of  $NO_X$  to  $SO_X$  emissions are higher than those in central and eastern USA In addition, the relatively dry climate in the Basin, favors the formation of  $HNO_3$  which occurs readily in the gas phase whereas much of the  $SO_2$  oxidation in other regions is believed to occur in cloud droplets.

Measurements of nitric acid (HNO<sub>3</sub>) by denuder tube technology are made on a routine basis in the Southern California acid deposition network. Recently, the HNO<sub>3</sub> results from a number of these stations have shown variability inconsistent with the expected behavior. It was, therefore, thought to be prudent to compare the measurements with a reference standard air monitoring technique at one of these sites in an attempt to identify the source of the variability.

In October 1993 the Research Division of the State of California Air Resources Board sponsored a four week comparison between the Tunable diode laser absorption spectrometer (TDLAS) and the denuder technique at the Southern California Air Quality Management monitoring site in Azusa, CA. Two denuder systems were employed in the study and they were situated within 10 ft of each other.

Tunable diode laser absorption spectroscopy (TDLAS) is a good choice for a reference standard for the following reasons [2]. Its high spectral resolution provides an unequivocal identification of the measured gaseous species free from interferences of other atmospheric constituents. In addition, the high sensitivity and rapid response of the TDLAS provides real time measurements with detection limits much better than those required for the ambient concentrations of most trace constituents under most atmospheric conditions.

Unisearch Associates Inc. used the TAMS-150 TDLAS designed for tropospheric air monitoring, to make real time measurements of HNO<sub>3</sub>. The detection limits of the TAMS-150 system were more than adequate for following the diurnal behavior of HNO<sub>3</sub> during the study period.

#### 2. EXPERIMENTAL

## 2.1 Principle of the TDLAS System

The TDLAS method takes advantage of the high monochromaticity and rapid tunability of Pb salt diode lasers to measure absorptions arising from single rotational-vibrational lines in the mid-infrared spectrum of a molecule. In order to facilitate the measurement of very low optical densities (<10.5) at line center and to reduce the chances of overlap between adjacent absorption lines, reduced pressures (~25 Torr) are used to minimize pressure broadening of the rotational lines. The atmospheric sample is pumped rapidly at the reduced pressure through a White cell which also provides the long optical path lengths (153 m) required to achieve the desired detection limits. The White cell is Teflon lined to minimize sticking of HNO<sub>3</sub> on the walls.

The technique of measuring HNO<sub>3</sub> by TDLAS has been described in detail by Hastie et al. [3] and a full description of the TAMS-150 field instrument may be found in the Unisearch Final Report to the State of California Air Resources Board, November 1987 [4] and in a paper by Mackay et al. [5].

## 2.2 Sampling and Calibration Procedures

Sample air was drawn through a 6 mm OD. 0.75 mm wall, PFA type Teflon tube approximately 4 m long. Particles were removed from the air by a 2 micron pore size Teflon filter located at the tubing entrance. A Teflon needle valve located 1 m upstream of the entrance to the White cell maintained the flow into the White cell at 10 standard liters per minute (SLM). The air traversed the inlet line in a few tenths of a second while the residence time in the White cell was about 4 seconds. The flow of air entering the White cell was monitored with a calibrated mass flowmeter just prior to each calibration and was adjusted by the needle valve as necessary. A motorized valve referenced to a MKS Baratron pressure gauge controlled the pressure in the White cell at 25 Torr.

The sensitivity of the TAMS-150 toward HNO<sub>3</sub> was determined by introducing a 'spike' of known concentration of the target gas to the air stream about 1 m upstream of the White cell entrance at a point immediately in front of (high pressure side) the Teflon needle valve. The concentration of the spike was chosen to provide mixing ratios similar to that of HNO<sub>3</sub> in the sampled air. In this way, any surface effects that may occur will be the same for the sampled and spiked air and should, therefore, cancel. A complete description of sampling integrity testing performed in the laboratory is described in Hastie et. al. [3]. Periodically, the sampling integrity of the rest (~3 m) of the sampling line was tested by introducing the spike at the sampling inlet in front of the particle filter. No differences were observed in the measured mixing ratio when the HNO<sub>3</sub> spike was added at the inlet or just up-stream of the White cell. The only difference noted was the time response (>80% change) to the added spike which was about 5 minutes when added at the inlet and less than 3 minutes when added at the needle valve.

Figure 1 demonstrates the response of the system to spike of nitric acid added to ambient air with and without the scrubber in place. The HNO<sub>3</sub> was added to the high pressure region of the sampling line ~1 meter upstream of the normal calibration injection point. With reference to Figure 1, after the system had been sampling ambient air which was at a level of about 3.5 ppbv, the Nylon scrubber used to obtain background spectra was interposed in the sampling line to scrub the sampled air of ambient nitric acid (BKGD). The measured signal was observed to drop to a value of about 1 ppbv after 5 minutes (background structure noise). A spike equivalent to 6.9 ppbv was then introduced and the signal rose to the expected level within 5 minutes. A second Nylon filter was then interposed into the sampling line immediately down stream of the HNO<sub>3</sub> spike injection point. The measured signal dropped to the previously measured background level within 5 minutes. Removal of the HNO<sub>3</sub> spike (at 09:42) showed no change in the measured background signal indicating that the Nylon filters effectively remove HNO<sub>3</sub> from the air stream. The response time is also shown to be of the order of 2-3 minutes and complete recovery of the HNO<sub>3</sub> spike is obtained

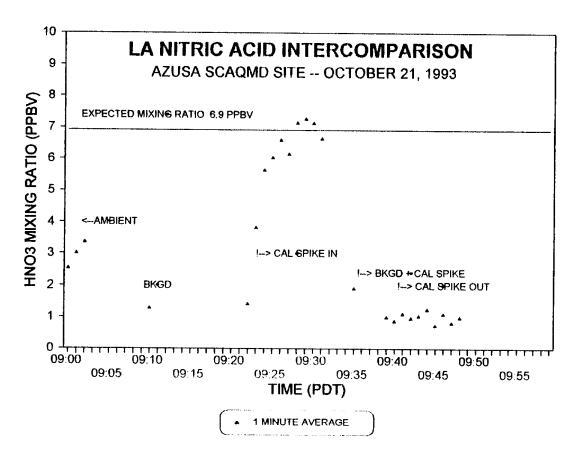


Figure 1: Response time of the TDLAS to a 6.9 ppbv spike of HNO<sub>3</sub> added into the ambient pressure side of the sampling line ~1 m upstream of the White Cell. Efficiency of the background scrubber is also demonstrated.

During the measurement periods the calibration gases flowed continuously through the addition lines. When not required for calibration, the gas mixture was exhausted far away from the inlet. During a calibration the addition line was inserted into the inlet line to introduce the calibration gas mixture to the sampled air stream. The addition point of the calibration spike was chosen for ease of calibration and as discussed above, to minimize the time required to stabilize before and after a calibration (~3 minutes).

The minimum detectable concentration, MDC, defined as a signal-to-noise ratio of 1, was determined experimentally at the selected laser operating condition. A 1 micron pore size Nylon filter was inserted into the sampling line at a point immediately upstream of the calibration gas inlet and the laser current scanned over the range of the absorption feature to obtain a background noise level,  $S_n$ . A known mixing ratio, MR, in ppbv of trace constituent is then added and the signal,  $S_s$  measured. The ratio of  $S_n/S_s$  X MR provides the MDC in ppbv, which for most of the time was about 0.5 ppbv for a 1 minute average and  $\sim$  50 -- 100 pptv for 1 hour averages.

The following description of the sequence of events during an automatic ambient air monitoring experiment illustrates how laser control, as well as data analysis, is achieved.

Information for the operating parameters selected for the HNO<sub>3</sub> measurements were input to the computer. The software then operated the system automatically. Under conditions when the ambient levels of HNO<sub>3</sub> were below 4 ppbv, a background spectrum was obtained by passing the air through the nylon filter every 30 minutes. Since the collection efficiency of the nylon filter was observed to be >80%, the mixing ratio of HNO<sub>3</sub> in the White cell was below the detection limit for levels below ~4 ppbv. The background spectrum was obtained and archived. Next, calibration gas was added to the scrubbed ambient air flow and, after a suitable stabilization period, a calibration-reference spectrum was obtained. The reference spectrum was also archived in its untreated form as were all subsequent spectra of ambient air. The background spectrum was subtracted (channel by channel) from the reference spectrum and the result normalized to the mean value of the untreated reference spectrum. This procedure essentially removes the frequency dependent structure present in the background from the reference spectra.

Under conditions where the HNO<sub>3</sub> mixing ratio was greater than 4 ppbv, no background subtraction was performed. The HNO<sub>3</sub> laser power was low enough that there was little frequency dependent laser noise. Eliminating the background subtraction procedure for concentrations above 4 ppbv did not introduce significant error in the analysis.

Figure 2 shows the data obtained on October 22, 1993 along with the measured background. The results show that the measured background is essentially at the detection limit during the night when the ambient HNO<sub>3</sub> levels are below 2 ppbv. The background increased during the day to about 1 ppbv when the HNO<sub>3</sub> reached a maximum of 13 ppbv for the 1 hour period 17:00 – 18:00. This is consistent with some point measurements made on October 30 with a nylon filter at the inlet. The nylon filter appears to trap >85% of the ambient nitric acid.

Some of the measured background signal shown in Figure 2 may be due to outgassing of HNO<sub>3</sub> from the walls of the White cell where it has accumulated during the ambient sampling period.

The measured signal was generally observed to decrease below the detection limit when the scrubber was left in the sampling line for longer periods (~15 minutes) although on occasion, a small residual signal ( $\leq 10\%$ ) was observed to persist even after 30 minutes. A second possible source of the measured background signal is that it may be due to dissociation of fine particle nitrate ( $< 2 \mu m$ ) at the reduced pressures in the White cell. This size fraction will not be collected by the Teflon inlet filter and most would also pass through the Nylon filter. Nevertheless, whichever is the case, it represents a very small (< 10%) error in the measurements.

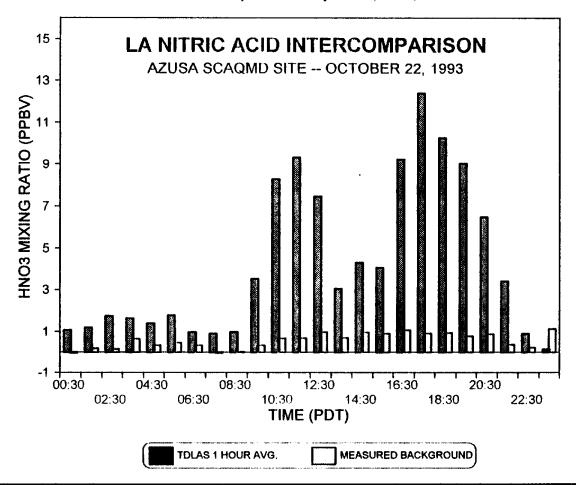


Figure 2: Diurnal variation in ambient HNO<sub>3</sub> and the measured background signal obtained by passing ambient air through a 1 μm pore size Nylon filter on October 22, 1993. Background measurements made every 15 minutes were combined to provide hourly average values.

Course particulate Nitrate (>2µm) did not appear to present a problem. The Teflon filter used to collect coarse particle matter at the inlet was changed each day and there was no evidence for a variation in the measured HNO<sub>3</sub> mixing ratio when the filter was changed. Also, HNO<sub>3</sub> was often observed to drop rapidly at sunset to near the detection limits. This would not be the case if particle nitrate were dissociating on the filter and bleeding HNO<sub>3</sub> into the sampled air. Furthermore, nighttime HNO<sub>3</sub> values would have been expected to be much higher if significant

dissociation was occurring as the decomposition would be favored during this period when the ambient gas phase HNO<sub>3</sub> was the lowest. Dissociation during the day should not be important as high HNO<sub>3</sub> would tend to force the equilibrium towards nitrate formation and not decomposition.

Once the calibration-background procedure was complete the software reset the solenoid valves to admit ambient air and, after an appropriate delay to achieve steady conditions (3 minutes), an ambient air spectrum was acquired. The background structure was subtracted (for mixing ratios below 4 ppbv).

The ambient air spectrum was then compared to the calibration spectrum using a least squares fitting procedure. Since the mean values of the calibration spectrum and the ambient air spectrum may differ due to potentially varying broad band transmittance of ambient air outside the White cell and since the mean value of the ambient spectrum contains no useful information, the calibration spectrum was adjusted to have a zero mean value before fitting. Thus, the intensity of the absorption line in the ambient air spectrum was obtained as a fraction of the calibration line intensity. Since shifting of the background spectra eventually reduces the integrity of the background spectrum, new background spectra are obtained at intervals determined by the operator (every 30 minutes on average).

During ambient air monitoring, spectra were obtained in one second blocks. These blocks of data were co-added and an average value of the ambient spectrum was obtained for the 1 minute integration time chosen. For each 1 second block the computer identified the spectral line center using the gas in the reference cell and shifted the ambient spectra as necessary to ensure accurate co-addition of spectra. When the reference spectrum was observe to have shifted by a significant number of channels (the spectrum is made up of 128 channels), which in this case was 3 channels, the computer commanded the temperature feedback circuit to adjust the laser temperature to restore the HNO<sub>3</sub> line center to coincide with the channel value employed during the calibration. This procedure results in greatly improved precision in the determination of the ambient mixing ratio.

# 2.3 HNO<sub>3</sub> Reference standard Calibration Procedures

The calibration spike was generated from a permeation device of our own design [3]. The HNO<sub>3</sub> permeation tube was constructed just prior to the field study and a permeation rate of ~280 ng/min. was measured in the laboratory with the NaOH standard to be employed in the field. The device was calibrated by titration against this standard NaOH solutions during the field study. In the field, two measurements were made with de ionized water brought from Unisearch and these gave results similar to that determined in the laboratory. Six measurements were made with de ionized water obtained from the local supermarket. Considerable difference was observed between the two sets of measurements. It appeared that the use of the de ionized water from the local store introduced an error in the on-site determination of the permeation rate. The measured titration end-point was found to be dependent on the volume of water employed. This suggested that something in the "de ionized" water was acting as a buffer. All of the determinations using local de ionized water provided permeation rates that were lower than the final, accepted rate, by 20% -- 40%. This error was not noted until the last week of the study.

One final determination was made with distilled water supplied by Cal Tech. The results were similar to those obtained with Unisearch distilled water. Table 1 summarizes the permeation rate measurements made prior to and during the field study.

In order to obtain an accurate determination of the permeation rate before the permeation system was turned off for the return trip, 6 samples were obtained in which the output of the permeation system was bubbled into various volumes of a basic aqueous solution for different bubbling times. This provided a wide range in the concentrations of the samples which were subsequently analyzed for  $NO_3$ - by Ion Chromatography at the ARB laboratories in Sacramento. Table 2 summarizes the results of these determinations. They provided an average value for the permeation rate of  $202 \pm 3$  ng.min.<sup>-1</sup>.

The permeation rate was also measured back at Unisearch after the study with a new NaOH standard. The results are provided in Table 3. Inspection of the three tables shows that the infield titrations with "good" distilled water (Table 1 # 1, 2 and 10) were about 20% higher than the values determined by the IC and the titrations after the study at Unisearch. It was subsequently discovered that the technician who produced the standard NaOH used in the field determinations had prepared the 0.1 M solution by weighing and not from a Reference Standard solution. As NaOH is very hydroscopic, the amount of NaOH weighed out would have been too low by the weight of water absorbed by the NaOH crystals, an error that could easily amount to 20%. These results (1, 2 and 10 in Table 1) are not, therefore included in the calculation of the average value. Results 1, 2 and 10 are very consistent, however, and provide strong evidence that the permeation rate did not change throughout the 1 month field study. The average permeation rate from all titrations was 198 ± 10 ng.min. in good agreement with the value obtained from the lon Chromatograph. The value employed for the analysis of the data, 200 ng.min. was calculated from the average of the results in Tables 2 and 3.

Table 1: Permeation rates for the Unisearch HNO<sub>3</sub> permeation device determined by titration against standard NaOH prepared prior to the field study using lab distilled water (1, 2, 3 and 10) and local store de ionized water (3 -- 9).

#	DATE	MOLES OF NaOH	VOLUME OF H <sub>2</sub> O (ml)	TRAP TIME (min.)	PERM. RATE (ng.min. <sup>-1</sup> )
1	August 19	5x 10 <sup>-6</sup>	20	1125	280
2	September 21	3x 10-	20	720	263
3	September 25	5x 10 <sup>-6</sup>	15	1220	258
4	October 13	2x 10 <sup>-6</sup>	10	1860	169
5	October 15	2x 10 <sup>-6</sup>	20	970	130
6	October 16	2x 10 <sup>-6</sup>	20	960	131
7	October 17	2x 10 <sup>-6</sup>	15	885	142
8	October 18	2x 10 <sup>-6</sup>	15	890	142
9	October 19	2x 10 <sup>-6</sup>	20	960	131
10	October 25	2x 10 <sup>-6</sup>	20	495	255

Table 2. Permeation rates for the Unisearch HNO<sub>3</sub> permeation device determined by Ion Chromatography from samples obtained during the field study.

SAMPLE	VOLUME OF ELUENT (ml)	TRAP TIME (min.)	CONCENTRATION (μg.ml <sup>-1</sup> )	PERM. RATE (ng.min. <sup>-1</sup> )
A	10	143	2.98	209
В	25	584	4.68	201
С	10	240	4.84	202
D	25	300	2.40	200
E	10	200	4.09	204
F	25	690	5.58	202
			AVERAGE	202±3

DATE	MOLES OF NaOH	VOLUME OF H <sub>2</sub> O (ml)	TRAP TIME (min.)	PERM. RATE (ng.min. <sup>-1</sup> )	WATER TYPE
November 12	2 x10 <sup>-6</sup>	20	636	198	de ionized
November 16	2x10 <sup>-6</sup>	20	654	193	de ionized
November 17	2x10 <sup>-6</sup>	20	637	198	distilled
November 23	2x10 <sup>-6</sup>	10	660	191	de ionized
November 24	2x10 <sup>-6</sup>	10	677	186	distilled
November 25	2x10 <sup>-6</sup>	20	662	190	distilled
November 27	2x10 <sup>-6</sup>	40	610	207	distilled
November 29	2x10 <sup>-6</sup>	60	570	221	distilled
November 30	4x10 <sup>-6</sup>	60	1260	200	distilled
			AVERAGE	198±10	

# 3. AMBIENT AIR MEASUREMENTS HNO<sub>3</sub>

## 3.1 Experimental Configuration

On September 29, 1993, the Unisearch mobile laboratory containing the TAMS-150 arrived at the Azusa SCAQMD monitoring station where the nitric acid measurements were to be made. The site is on the edge of a mixed residential/industrial area at the base of the San Gabriel mountains which are to the north. The Glendora Canyon empties into this area several miles to the east. Dr. Gervase I. Mackay and Dr. David R. Karecki from Unisearch shared the operation of the TAMS-150 during the study. The TAMS-150 was configured for single measurements of HNO<sub>3</sub> with a 1 minute integration time. The mobile laboratory was positioned at the north end of the SCAQMD building which housed the nitric acid denuders on its roof.

The inlet systems used in this study was constructed entirely of PFA Teflon fittings and tubing. The sampling port was positioned on the roof of the building at approximately the same height as the denuder sampler inlets some 1 m above the roof ( $\sim$ 3 m above the ground) and about 5 m away from the nearest denuder system. The second denuder was located about 2 m from the first. The TDLAS inlet tube consisted of 4 m of 6 mm OD, 0.75 mm wall PFA Teflon tubing. A filter holder containing a  $2\mu m$  pore size Teflon filter was installed at the sampling end of the line. This filter was replaced daily between 07:00 and 09:00.

#### 3.2 Measurement Procedure

The TAMS-150 obtained data points every minute. The raw data were stored on floppy diskettes for future analysis in the laboratory and the real time measurements were printed out at 1 minute intervals. Calibrations were performed at least 4 times a day at operator chosen intervals. The sensitivity of the instrument toward HNO<sub>3</sub> never varied by more than 10% and the changes were random in nature. Backgrounds were usually obtained every 30 minutes and on occasion at more frequent intervals.

The accuracy of the measurements is estimated to be  $\pm$  15%. Three sources of error contribute to the overall accuracy; Calibration errors, Precision and Optical alignment variations which contribute to changes in the sensitivity of the instrument between calibrations. The major source of calibration error was the standardization of the permeation device (pH or IC) which has an uncertainty assessed at 5%. Additional uncertainties of  $\pm$  2% are caused by temperature variations of the permeation device, and  $\pm$  1% from the measurement of the total gas flow into which the HNO<sub>3</sub> spike was added. The flowmeter (Tylan, model FM360-20SLM) was calibrated against a dry test meter prior to the study with agreement within 1%. The precision of the instrument has been determined empirically to be better than 1% and the long term variability of the sensitivity between calibrations was observed to be within 7%.

Data coverage was excellent. A total of 30 ½ days of measurements were obtained. Only 15 hours out of a total of 732 hours were lost due to instrument malfunction. Less than 10 minutes of any hour was lost due to calibration periods and this occurred on average only 4 times per day. Usually only one calibration was made during the hours of comparison with the denuders.

### 4. RESULTS AND DISCUSSION

The measurement period was 12:00, September 30, through 24:00, October 30, 1993 inclusive. Data points were obtained over 1 minute averaging periods. The one minute HNO<sub>3</sub> data were re-analyzed into hourly average values at Unisearch. During the first 12 days of the study the system was not performing optimally and the detection limit for 1 hour averages was in the range 0.3 -- 0.5 ppbv. After October 12, a better absorption feature was identified and the detection limit was much better, in the range 50 -- 100 pptv. Nevertheless, the mixing ratios were well above the detection limit during the daytime comparison period of 10:00 -- 18:00 throughout the study. The results are presented in tabular form in Appendix A which contains the 1 hour average values (determined on the half hour) for HNO<sub>3</sub> over the entire study.

Figure 3 shows the results obtained on October 25 which were typical of the observations for most days of the study. On a few occasions HNO<sub>3</sub> exhibited two peaks (see Figure 2).

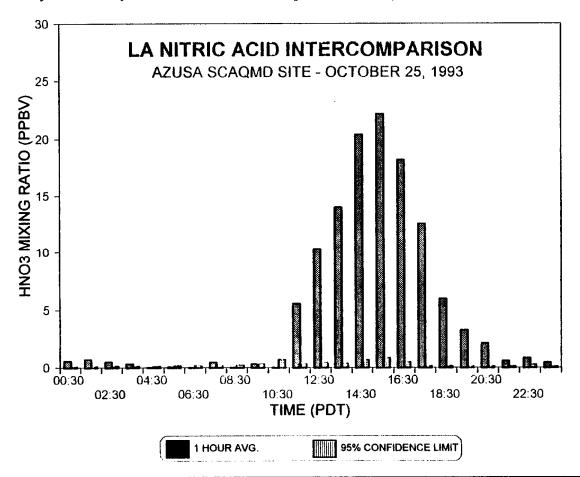


Figure 3: Diurnal variation in the one hour average ambient HNO<sub>3</sub> measured by the TDLAS on October 25, 1993. The lower trace is the calculated hourly average confidence limit which is comparable to the minimum detection limit for that period.

Figure 4 shows the variation in the ambient HNO<sub>3</sub> mixing ratio measured by the TAMS-150 during the entire study period. The diurnal behavior was quite regular. The maximum concentrations occurred between 12.00 and 18.00 each day with most peaking in the 15.00 -- 16.00 hourly period. Nighttime levels were generally in the 0.2 -- 1 ppbv range. On occasion HNO<sub>3</sub> reached the instrument detection limit at nighttime (even after improved detection limits of <100 pptv were obtained -- see Figure 3) while at other times the nighttime levels remained high, in the 2 -- 4 ppbv range.

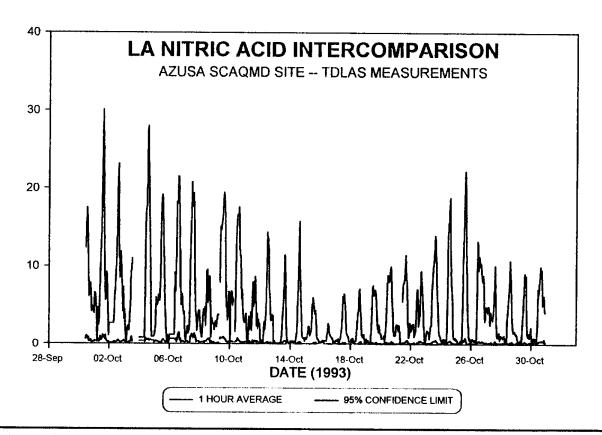


Figure 4: Diurnal variation in the one hour average ambient HNO<sub>3</sub> measured by the TDLAS during the period 12:00, September 30, 1993, through 24:00, October 30, 1993. The lower trace is the calculated hourly average confidence limit which is comparable to the minimum detection limit for that period.

The HNO<sub>3</sub> daily maximum was observed to decrease from ~30 ppbv on September 30 to only 3 ppbv on October 16. The decrease was gradual until October 15 when the levels abruptly dropped from 15 ppbv on the October 14 to 6 ppbv on October 15 and only 3 ppbv on October 16. During this latter period the weather was unsettled, with morning fog and occasional rain. After October 16 the weather improved, being mostly sunny, and the HNO<sub>3</sub> levels increased slowly to a maximum of 22 ppbv on October 25. After that, the daily maximum remained about 10 ppbv for the rest of the study. It should be noted that the last 5 days of the study overlapped the major forest fires in the Los Angeles area.

The daily average HNO<sub>3</sub> measured by the TDLAS along with the measured uncertainty is summarized in Table 4 and shown graphically in Figure 5. The 24 hr average HNO<sub>3</sub> mixing ratio measured by the TDLAS showed considerable variability particularly during the first two weeks of the study. As was observed with the daily maximum values, the 24 hour average value showed a minimum value on October 16. Prior to that, the levels varied between ~ 9 ppbv and 4 ppbv although a general decrease was observed on a daily basis after October 12. The daily average increased again after the October 16 maximizing at about 5 ppbv over the period October 22 through October 25 after which it again slowly decreased.

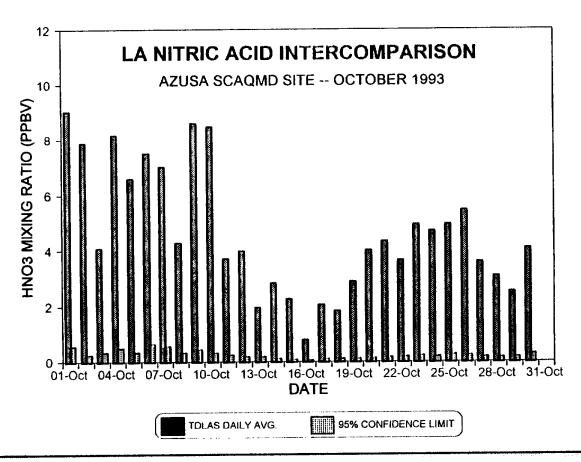


Figure 5: Daily average HNO<sub>3</sub> mixing ratios measured by the TDLAS during the period 00:00, October 1, 1993, through 24:00, October 30, 1993. The lower trace is the calculated daily average confidence limit which is comparable to the minimum detection limit for that period

The average HNO<sub>3</sub> mixing ratios and the 95% confidence limits measured during the daytime period, 10:00 through 18:00 PDT, are summarized in Table 5. The results are shown graphically in Figure 6. The daytime averages showed much the same behavior as the daily averages. The maximum value of ~20 ppbv was reached on October 4 and the minimum value of 1.5 ppbv for the daytime average was observed on October 16. The HNO<sub>3</sub> daytime mixing ratio showed a decline from the highest values in early October to a minimum on the October 16 after which the

HNO<sub>3</sub> increased again to a high of almost 13 ppbv on October 25. After October 25 the HNO<sub>3</sub> again slowly decreased.

Table 6 shows the average HNO<sub>3</sub> measured during the non-comparison "nighttime" period 18:00 at night through 10:00 the next morning for each 24 hour period. Also shown is the ratio of the nighttime to daytime measurements. This ratio varies from a high of 59% on October 27 to a minimum of 4% on October 13. There is no correlation in the ratio with maximum daily mixing ratio. Furthermore, there does not appear to be a correlation with weather conditions insofar as humidity, precipitation and solar radiation are concerned. It suggests that air circulation, wind direction, wind speed and air trajectory must be the cause of the variation in this ratio and the higher nighttime mixing ratios observed on occasion. The meteorological data, however, is not currently available for comparison and possible confirmation of this hypothesis.

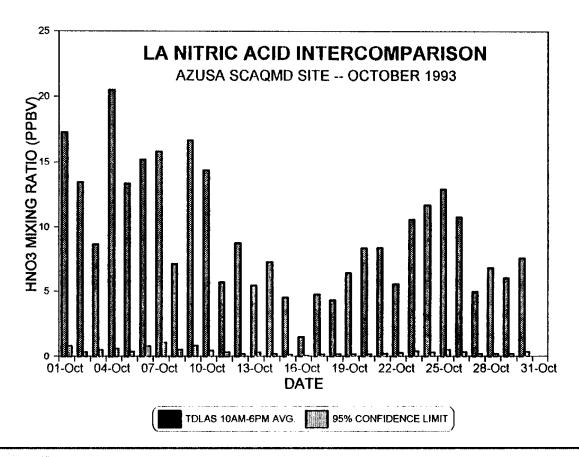


Figure 6: Daytime (10:00 -- 18:00) average HNO<sub>3</sub> mixing ratios measured by the TDLAS during the period 00:00, October 1, 1993, through 24:00, October 30, 1993. The lower trace is the calculated daytime average confidence limit which is comparable to the minimum detection limit for that period

Table 4 Daily average HNO<sub>3</sub> mixing ratio measured by the TDLAS during the LA Acid Precipitation Intercomparison Study October 1 -- 30, 1993 at the Azusa SCAQMD site.

DATE DD-MM	START TIME PDT	END TIME PDT	MIXING RATIO (PPBV)	95% LIMIT (PPBV)	COMMENTS
01-Oct	00:00	23:59	9.01	0.56	
02-Oct	00:00	23:59	7.86	0.24	
03-Oct	00:00	23:59	4.08	0.32	DATA MISSING 14:00 24:00
04-Oct	00:00	23:59	8.16	0.49	
05-Oct	00:00	23:59	6.58	0.33	
06-Oct	00:00	23:59	7.50	0.64	
07-Oct	00:00	23:59	7.01	0.57	
08-Oct	00:00	23:59	4.26	0.33	
09-Oct	00:00	23:59	8.58	0.44	DATA MISSING 08:00 09:00
10-Oct	00:00	23:59	8.46	0.31	DATA MISSING 07:00 09:16
11-Oct	00:00	23:59	3.70	0.23	
12-Oct	00:00	23:59	3.97	0.18	
13-Oct	00:00	23:59	1.95	0.18	
14-Oct	00:00	23:59	2.83	0.11	
15-Oct	00:00	23:59	2.27	0.08	
16-Oct	00:00	23:59	0.78	0.06	
17-Oct	00:00	23:59	2.06	0.10	
18-Oct	00:00	23:59	1.83	0.10	
19-Oct	00:00	23:59	2.88	0.11	
20-Oct	00:00	23:59	3.99	0.13	
21-Oct	00:00	23:59	4.33	0.17	DATA MISSING 09:00 11:14
22-Oct	00:00	23:59	3.64	0.19	
23-Oct	00;00	23:59	4.94	0.22	
24-Oct	00:00	23:59	4.71	0.20	
25-Oct	00:00	23:59	4.95	0.27	
26-Oct	00:00	23:59	5.46	0.23	
27-Oct	00:00	23:59	3.59	0.17	
28-Oct	00:00	23:59	3.07	0.15	
29-Oct	00:00	23:59	2.52	0.16	
30-Oct	00:00	23:59	4.08	0.29	STUDY END 24:00

Table 5 Daytime (10:00 -- 18:00) average HNO<sub>3</sub> mixing ratio measured by the TDLAS during the LA Acid Precipitation Intercomparison Study October 1 -- 30, 1993 at the Azusa SCAQMD site.

DATE DD-MM	START TIME PDT	END TIME PDT	MIXING RATIO (PPBV)	95% LIMIT (PPBV)	COMMENTS
01-Oct	10:00	18:00	17.25	0.81	
02-Oct	10:00	18:00	13.40	0.31	
03-Oct	10:00	18:00	8.64	0.51	DATA MISSING 14:00 18:00
04-Oct	10:00	18:00	20.48	0.59	
05-Oct	10:00	18:00	13.32	0.37	
06-Oct	10:00	18:00	15.18	0.79	
07-Oct	10:00	18:00	15.80	1.07	
08-Oct	10:00	18:00	7.09	0.53	
09-Oct	10:00	18:00	16.66	0.83	
10-Oct	10:00	18:00	14.34	0.44	
11-Oct	10:00	18:00	5.67	0.32	
12-Oct	10:00	18:00	8.72	0.20	
13-Oct	10:00	18:00	5.44	0.31	
14-Oct	10:00	18:00	7.22	0.19	
15-Oct	10:00	18:00	4.52	0.14	
16-Oct	10:00	18:00	1.49	0.05	
17-Oct	10:00	18:00	4.75	0.15	
18-Oct	10:00	18:00	4.30	0.17	
19-Oct	10:00	18:00	6.37	0.16	
20-Oct	10:00	18:00	8.32	0.17	
21-Oct	10:00	18:00	8.34	0.22	DATA MISSING 10:00 11:14
22-Oct	10:00	18:00	5.52	0.26	
23-Oct	10:00	18:00	10.55	0.40	
24-Oct	10:00	18:00	11.65	0.31	
25-Oct	10:00	18:00	12.86	0.50	
26-Oct	10:00	18:00	10.74	0.32	
27-Oct	10:00	18:00	4.94	0.19	
28-Oct	10:00	18:00	6.76	0.18	
29-Oct	10:00	18:00	6.00	0.20	
30-Oct	10:00	18:00	7.56	0.36	STUDY END 24:00

Table 6 Average HNO<sub>3</sub> mixing ratio for the non-daytime averaging period (18:00 -- 10:00) measured by the TDLAS during the LA Acid Precipitation Intercomparison Study October 1 -- 30, 1993 at the Azusa SCAQMD site.

DATE	START	END	MIXING	95%	RATIO
DD-MM	TIME	TIME	RATIO	LIMIT	18:00 - 10:00
	PDT	PDT	(PPBV)	(PPBV)	10:00 - 18:00
01-Oct	18:00	10:00	4.89	0.43	0.28
02-Oct	18:00	10:00	5.09	020	0.38
03-Oct	18:00 -	10:00	2.25	0.25	0.26
04-Oct	18:00	10:00	2.00	0.44	0.10
05-Oct	18:00	10:00	3.21	0.31	0.24
06-Oct	18:00	10:00	3.66	0.57	0.23
07-Oct	18:00	10:00	2.61	0.32	0.17
08-Oct	18:00	10:00	2.85	0.23	0.40
09-Oct	18:00	10:00	4.28	0.23	0.26
10-Oct	18:00	10:00	5.10	0.23	0.36
11-Oct	18:00	10:00	2.71	0.26	0.48
12-Oct	18:00	10:00	1.59	0.17	0.18
13-Oct	18:00	10:00	0.21	0.11	0.04
14-Oct	18:00	10:00	0.64	0.07	0.09
15-Oct	18:00	10:00	1.14	0.05	0.25
16-Oct	18:00	10:00	0.42	0.07	0.28
17-Oct	18:00	10:00	0.71	0.07	0.15
18-Oct	18:00	10:00	0.60	0.07	0.14
19-Oct	18:00	10:00	1.14	0.09	0.18
20-Oct	18:00	10:00	1.83	0.11	0.22
21-Oct	18:00	10:00	2.45	0.14	0.29
22-Oct	18:00	10:00	2.70	0.15	0.49
23-Oct	18:00	10:00	2.14	0.13	0.20
24-Oct	18:00	10:00	1.24	0.14	0.11
25-Oct	18:00	10:00	1.00	0.15	0.08
26-Oct	18:00	10:00	2.82	0.18	0.26
27-Oct	18:00	10:00	2.92	0.16	0.59
28-Oct	18:00	10:00	1.23	0.14	0.18
29-Oct	18:00	10:00	0.78	0.14	0.13
30-Oct	18:00	10:00	2.35	0.25	0.31

## 4. CONCLUSIONS

Measurements of HNO<sub>3</sub> by the TDLAS were made during the period 12:00, September 30, 1993 through 24:00, October 30, 1993 inclusive. Data was obtained over 1 minute averaging periods. The results were reduced to 1 hour average values and Daytime average value (10:00 -- 18:00) for comparison with measurements made by the ARB denuder samplers. Data coverage was better than 98% and detection limits of better than 0.2 ppbv were obtained for the one hour averages.

The diurnal behavior of HNO<sub>3</sub> was quite regular. The maximum concentrations generally occurred between 14:00 and 16:00 each day. The HNO<sub>3</sub> daily maximum varied between 3 ppbv (during wet weather) and 30 ppbv (hot dry weather) with the median value of about 15 ppbv for the entire period. The values calculated for the period 10:00 - 18:00 (the denuder sampling period) were on average twice the nighttime (18:00 - 10:00) values and represented ~75% of the total daily HNO<sub>3</sub> burden. This indicates that, on most occasions, the denuders should capture a major fraction of the HNO<sub>3</sub> produced during a 24 hour period.

Tests performed during the field study indicated that there were no significant losses of HNO<sub>3</sub> in the sampling line, the sampling integrity was good and the scrubbing efficiency of the Nylon filters used to remove HNO<sub>3</sub> from ambient air to allow background noise determinations was adequate for HNO<sub>3</sub> levels below ~5 ppbv. Furthermore, there was no evidence for any large particle nitrate (>2  $\mu$ m) dissociation from the particulate matter collected on the inlet filter contributing to the HNO<sub>3</sub> signal measured by the TDLAS. While it could not be completely ruled out, dissociation of small nitrate particles (<2  $\mu$ m) (which passed through the filter) in the White cell was not obvious and the results indicate that it could contribute at most 10% of the measured signal at any time.

## 5. REFERENCES

- 1. The Atmospheric Acidity Protection Program: Annual Report to the Governor and the Legislature, (1992)
- 2. H. I. Schiff, G. W. Harris, G. I. Mackay, "Tunable Diode Laser Absorption Spectrometry as a Reference Method for Tropospheric Measurements", Commission of the European Communities Air Pollution Research Reports: Monitoring of Gaseous Pollutants by Tunable Diode Lasers-II, Mainz, FRG, (October 1988)
- 3. D. R. Hastie, H. I. Schiff, G. I. Mackay, T. Iguchi, B. A. Ridley, "Tunable Diode Laser Systems for Measuring Trace Gases in Tropospheric Air", Environmental Science and Technology 17, 352 (1984)
- 4. Unisearch Final Report to the State of California Air Resources Board contract number A5-189-32 (1987)
- 5. G. I. Mackay, L. K. Mayne, H. I. Schiff, "Measurements of H<sub>2</sub>O<sub>2</sub> and HCHO by Tunable Diode Laser Absorption Spectroscopy During the 1986 Carbonaceous Species Methods Comparison Study in Glendora, California" Aerosol Sci. & Technol. 12, 56-63 (1990)

# APPENDIX A

1 Hour average HNO<sub>3</sub> mixing ratios

	·		
J			
		,	
	•	,	

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS
SPECIES: HNO3 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE DD-MMM-YY	START TIME PDT	END TIME PDT	MIXING RATIO (PPBV)	95% LIMIT (PPBV)	CORR.	COMMENTS
30-Sep	00:00	01:00				
30-Sep	01:00	02:00				
30-Sep	02:00	03:00				
30-Sep	03:00	04:00				
30-Sep	04:00	05:00				
30-Sep	05:00	06:00				
30-Sep	06:00	07:00				
30-Sep	07:00	08:00				
30-Sep	08:00	09:00				
30-Sep	09:00	10:00				
30-Sep	10:00	11:00				
30-Sep	11:00	12:00				
30-Sep	12:00	13:00	12.297	0.679	0.97	MEASUREMENTS BEGAN @ 12:00
30∼Sep	13:00	14:00	15.063	1.101	0.95	
30-Sep	14:00	15:00	17.537	0.955	0.97	
30-Sep	15:00	16:00	15.535	0.719	0.98	
30-Sep	16:00	17:00	10.211	0.867	0.93	
30-Sep	17:00	18:00	6.081	0.301	0.97	
30-Sep	18:00	19:00	7.055	0.486	0.95	
30-Sep	19:00	20:00	7.847	0.306	0.98	
30-Sep	20:00	21:00	7.782	0.580	0.95	
30-Sep	21:00	22:00	4.202	0.267	0.96	
30-Sep	22:00	23:00	4.914	0.133	0.99	
30-Sep	23:00	24:00	4.787	0.336	0.95	
01~0ct	00:00	01:00	3.972	0.233	0.97	
01-0ct	01:00	02:00	6.617	0.437	0.96	
01-0ct	02:00	03:00	6.549	0.401	0.96	
01-0ct	03:00	04:00	5.524	0.376	0.95	
01-0ct	04:00	05:00	4.088	0.475	0.88	
01-0ct	05:00	06:00	0.656	0.220	0.54	
01-0ct	06:00	07:00	2.573	0.684	0.63	
01-0ct	07: <b>0</b> 0	08:00	4.748	0.580	0.87	CALIBRATION 07:34 - 07:57
01-0ct	08:00	09:00	2.515	0.254	0.81	
01-0ct	09:00	10:00	6.807	0.431	0.91	
01-0ct	10:00	11:00	9.971	1.008	0.96	
01-0ct	11:00	12:00	12.663	0.553	0.91	
01-0ct	12:00	13:00	14.735	0.515	0.98	CALIBRATION 12:42 - 12:49
01-0ct	13:00	14:00	23.432	0.682	0.99	
01-0ct	14:00	15:00	30.096	1.199	0.99	
01-0ct	15:00	16:00	24.421	1.023	0.98	
01-0ct	16:00	17:00	15.201	0.806	0.98	
01-0ct	17:00	18:00	7.474	0.667	0.97	£
01-0ct	18:00	19:00	5.628	1.140	0.92	
01-0ct	19:00	20:00	5.944	0.479		CALIBRATION 19:36 - 19:47
01-0ct	20:00	21:00	9.248	0.483	0.94	
01-0ct	21:00	22:00	7.755	0.246	0.97	
01-0ct	22:00	23:00	4.484	0.184	0.99	
01-0ct	23:00	24:00	1.128	0.248	0.98	

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS

SPECIES: HN03 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE DD-MMM-YY	START TIME PDT	END TIME PDT	MIXING RATIO (PPBV)	95% LIMIT (PPBV)	CORR.	COMMENTS
=======================================	========				=======	
02-0ct	00:00	01:00	2.716	0.134		NOISY SIGNAL
02-0ct	01:00	02:00	2.716	0.134		AVERAGE 00:00 - 08:00
02-0ct	02:00	03:00	2.716	0.134	0.98	AVERAGE 00:00 - 08:00
02-0ct	03:00	, 04:00	2.716	0.134	0.98	
02-0ct	04:00	05:00	2.716	0.134	0.98	
02-0ct	05:00	06:00	2.716	0.134	0.98	
02-0ct	06:00	07:00	2.716	0.134	0.98	
02-0ct	07:00	08:00	2.716	0.134		CALIBRATION 07:39 - 07:55
02-0ct	08:00	09:00	3.905	0.304	0.95	07.00
02-0ct	09:00	10:00	6.327	0.135	1.00	
02-0ct	10:00	11:00	6.733	0.183	0.99	
02-0ct	11:00	12:00	9.334	0.220	0.99	
02-0ct	12:00	13:00	10.299	0.269	0.99	
02-0ct	13:00	14:00	14.594	0.240	1.00	
02-0ct	14:00	15:00	21.013	0.509	0.99	
02-0ct	15:00	16:00	23.128	0.495	1.00	
02-0ct	16:00	17:00	13.613	0.348	0.99	
02-0ct	17:00	18:00	8.467	0.256	0.99	
02-0ct	18:00	19:00	9.499	0.185	1.00	
02~0ct	19:00	20:00	11.878	0.149	1.00	
02-0ct	20:00	21:00	9.611	0.265	0.99	
02-0ct	21:00	22:00	6.847	0.338	0.98	
02-0ct	22:00	23:00	4.190	0.275	0.96	
02-0ct	23:00	24:00	7.378	0.480	0.96	
03-0ct	00:00	01:00	3.235	0.491	0.82	CALIBRATION 00:50 - 01:02
03-0ct	01:00	02:00	4.429	0.231	0.97	
03-0ct	02:00	03:00	1.890	0.421	0.70	
03-0ct	03:00	04:00	0.524	0.369	0.29	
03~0ct	04:00	05:00	0.324	0.143	0.44	
03-0ct	05:00	06:00	1.919	0.182	0.92	•
03-0ct	06:00	07:00	2.376	0.115	0.98	
03-0ct	07:00	08:00	2.159	0.163	0.94	
03-0ct	08:00	09:00	1.732	0.203	0.88	
03-0ct	09:00	10:00	3.897	0.164		CALIBRATION 09:28 - 09:34
03-0ct	10:00	11:00	4.773	0.424	0.93	
03-0ct	11:00	12:00	9.187	0.382	0.98	
03-0ct	12:00	13:00	9.620	0.971	0.91	****
03-Oct 03-Oct	13:00	14:00	10.993	0.277	0.99	CALIBRATION 13:44 - 14:13
03-0ct	14:00	15:00				SYSTEM LEFT IN CALIBRATION
03-0ct	15:00 16:00	16:00 17:00				MODE. NO DATA 14:00-24:00
03-0ct	17:00	18:00				
03-0ct	18:00	19:00				
03-0ct	19:00	20:00				
03-0ct	20:00	21:00				
03-0ct	21:00	22:00				
03-0ct	22:00	23:00				
03-0ct	23:00	24:00				
<b>-</b>						

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS
SPECIES: HN03 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE DD-MMM-YY	START TIME	END Time	MIXING RATIO	95% Limit	CORR.	COMMENTS			
	PDT	PDT	(PPBV)	(PPBV)					
***************************************									
04-0ct	00:00	01:00	0.857	0.403	0.43	CALIBRATION LEFT ON			
04-0ct	01:00	02:00	0.857	0.403	0.43	AVERAGE DATA 00:00 - 09:00			
04-0ct	02:00	03:00	0.857	0.403	0.43				
04-0ct	03:00	04:00	0.857	0.403	0.43				
04-0ct	04:00	05:00	0.857	0.403	0.43				
04-0ct	05:00	06:00	0.857	0.403	0.43				
04-0ct	06:00	07:00	0.857	0.403	0.43				
04-0ct	07:00	08:00	0.857	0.403	0.43	CALIBRATION 07:51 - 08:39			
04-0ct	08:00	09:00	0.857	0.403	0.43				
04-0ct	09:00	10:00	4.139	0.245	0.97				
04-0ct	10:00	11:00	15.250	0.801	0.94				
04-0ct	11:00	12:00	17.216	0.530	0.97				
04-0ct	12:00	13:00	17.768	0.661	0.99				
04-0ct	13:00	14:00	27.221	0.616	0.99				
04-0ct	14:00	15:00	28.024	0.523	1.00				
04-0ct	15:00	16:00	24.134	0.671	0.99				
04-0ct	16:00	17:00	19.045	0.426	0.99				
04-0ct	17:00	18:00	15.169	0.501	0.99				
04-0ct	18:00	19:00	12.359	0.614	0.98				
04-0ct	19:00	20:00	3.697	0.576	0.82				
04-0ct	20:00	21:00	1.014	0.482	0.42	AVERAGE VALUE 20:00 - 24:00			
04-0ct	21:00	22:00	1.014	0.482	0.42				
04-0ct	22:00	23:00	1.014	0.482	0.42	CALIBRATION 22:35 -23:03			
04-0ct	23:00	24:00	1.014	0.482	0.42				
05-0ct	00:00	01:00	1.161	0.181	0.75				
05-0ct	01:00	02:00	1.529	0.294	0.67				
05-0ct	02:00	03:00	2.528	0.446	0.70				
05-0ct	03:00	04:00	6.017	0.470	0.91				
05-0ct	04:00	05:00	5.034	0.321	0.94				
05-0ct	05:00	06:00	5.058	0.326	0.94				
05-0ct	06:00	07:00	5.404	0.280	0.96				
05-0ct	07:00	08:00	6.362	0.267		CALIBRATION 07:41 - 07:57			
05-0ct 05-0ct	08:00	09:00	5.819	0.213	0.98				
05-0ct	09:00	10:00	5.585	0.213	0.98				
05-0ct	10:00	11:00	8.605	0.149	1.00				
05-0ct	11:00	12:00	15.070	0.208	1.00				
05-0ct	12:00	13:00	18.782	0.198	1.00				
05-0ct	13:00 14:00	14:00	19.168	0.499	0.99				
05-0ct	15:00	15:00 16:00	17.130	0.630	0.98				
05-0ct	16:00	17:00	12.978 9.469	0.570	0.97				
05-0ct	17:00	18:00		0.418	0.97	041 IDDATEOU 4 T 00			
05-0ct	18:00	19:00	5.376 3.082	0.302		CALIBRATION 17:23 - 17:42			
05-0ct	19:00	20:00	1.640	0.131	0.97				
05-0ct	20:00	21:00	0.501	0.166	0.87				
05-0ct	21:00	22:00	1.211	0.566	0.15				
05-0ct	22:00	23:00	-0.072	0.510	0.38	CALIBRATION OD OD OF 15			
05-Oct	23:00	24:00	0.485	0.322		CALIBRATION 22:30 - 22:43			
		27.00	0.405	0.228	0.35				

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS

SPECIES: HN03 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE DD-MMM-YY	START TIME	END Time	MIXING RATIO	95% LIMIT	CORR.	COMMENTS
	PDT	PDT	(PPBV)	(PPBV)		
=======================================					*=======	
06-0ct	00:00	01:00	1.260	0.700	0.66	AVERAGE 00:00 - 09:00
06-0ct	01:00	02:00	1.260	0.700	0.66	
06-Oct	02:00	03:00	1.260	0.700	0.66	
06-Oct	03:00	2 04:00	1.260	0.700	0.66	
06-0ct	04:00	05:00	1.260	0.700	0.66	
06-Oct	05:00	06:00	1.260	0.700	0.66	
06-0ct	06:00	07:00	1.260	0.700	0.66	
06-0ct	07:00	08:00	1.260	0.700	0.66	CALIBRATION 07:44 - 08:10
06-0ct	08:00	09:00	1.260	0.700	0.66	•
06-0ct	09:00	10:00	9.206	0.621	0.95	
06-Oct	10:00	11:00	6.718	0.689	0.90	
06-0ct	11:00	12:00	11.615	0.262	0.99	
06-0ct	12:00	13:00	18.300	0.477	0.99	
06-0ct	13:00	14:00	18.065	1.060	0.96	
06-0ct	14:00	15:00	21.493	1.356	0.96	
06-0ct	15:00	16:00	21.421	1.492	0.95	
06-0ct	16:00	17:00	16.684	0.507	0.99	
06-0ct	17:00	18:00	7.166	0.473	0.96	
06-0ct	18:00	19:00	11.979	0.735	0.96	CALIBRATION 18:02 - 18:23
06-0ct	19:00	20:00	5.009	0.206	0.98	
06-0ct	20:00	21:00	6.199	0.223	0.99	
06-Oct	21:00	22:00	6.448	0.379	0.96	
<b>0</b> 6-0ct	22:00	23:00	4.446	0.302	0.95	CALIBRATION 22:50 - 23:05
06-0ct	23:00	24:00	3.879	0.298	0.94	
07-0ct	00:00	01:00	4.192	0.193	0.98	
07-0ct	01:00	02:00	1.265	0.237	0.76	
07-0ct	02:00	03:00	0.517	0.276	0.38	
07-0ct	03:00	04:00	1.395	0.408	0.60	
07-0ct	04:00	05:00	1.433	0.428	0.59	
07-0ct	05:00	06:00	2.333	0.280	0.88	
07-0ct	06:00	07:00	1.319	0.182	0.84	
07-0ct	07:00	08:00	1.898	0.093		CALIBRATION 07:33 - 07:53
07-0ct	08:00	09:00	1.808	0.172	0.92	
07-0ct	09:00	10:00	4.988	0.133	0.99	
07-0ct	10:00	11:00	12.086	0.999	0.93	
07-0ct	11:00	12:00	16.576	1.224	0.95	
07-0ct	12:00	13:00	20.792	1.304	0.96	
07-0ct	13:00	14:00	17.961	0.839	0.98	
07-0ct 07-0ct	14:00 15:00	15:00	17.591	0.769	0.98	
07-0ct	16:00	16:00	19.392	1.136	0.97	
07-0ct	17:00	17:00 18:00	14.813 7.168	1.385	0.92 0.86	
07-0ct	18:00	19:00	4.375	0.907		CALIBRATION 18:05 - 18:23
07-0ct	19:00	20:00	3.482	0.265		CALIBRATION GAS LEFT ON
07-0ct	20:00	21:00	1.719	0.203		18:23 - 22:27
07-0ct	21:00	22:00	2.859	0.437		CALIBRATION GAS SUBTRACTED
07-0ct	22:00	23:00	3.850	0.376	0.96	CHEZONALIZON OND GUDIRACIEU
07-0ct	23:00	24:00	4.351	0.344	0.94	

LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS
SPECIES: HN03 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE DD-MMM-YY	START TIME	END TIME	MIXING RATIO	95% LIMIT	CORR.	COMMENTS
	PDT	PDT	(PPBV)	(PPBV)		
08-0ct 08-0ct	00:00	01:00	4.317	0.182	0.98	
08-0ct	01:00 02:00	02:00 03:00	2.680 1.722	0.167 0.177	0.96 0.90	
08-0ct	03:00	04:00	1.103	0.267	0.67	
08-0ct	04:00	05:00	0.906	0.254	0.61	
08-0ct	05:00	06:00	2.397	0.222	0.92	
08-0ct	06:00	07:00	4.147	0.233	0.97	
08-0ct	07:00	08:00	4.500	0.138		CALIBRATION 07:43 - 08:10
08-0ct	08:00	09:00	3.711	0.342	0.92	0.220
08-0ct	09:00	10:00	4.762	0.304	0.96	
08-0ct	10:00	11:00	2.382	0.412	0.78	
08-0ct	11:00	12:00	5.507	0.349	0.96	
08-0ct	12:00	13:00	9.443	0.590	0.96	
08-0ct	13:00	14:00	9.572	0.589	0.96	
08-0ct	14:00	15:00	5.220	0.741	0.84	
08-0ct	15:00	16:00	7.520	0.554	0.95	
08-0ct	16:00	17:00	8.755	0.760	0.93	
08-0ct	17:00	18:00	8.336	0.206	0.99	
08-0ct	18:00	19:00	0.935	0.407	0.45	CALIBRATION 18:11 - 18:20
08-0ct	19:00	20:00	3.030	0.198	0.96	
08-0ct	20:00	21:00	3.364	0.222	0.96	
08-0ct	21:00	22:00	2.715	0.203	0.95	
08-0ct	22:00	23:00	2.556	0.108	0.98	CALIBRATION 22:35 - 22:53
08-0ct	23:00	24:00	2.674	0.227	0.93	
09-0ct	00:00	01:00	1.883	0.112	0.97	
09-0ct	01:00	02:00	2.292	0.107	0.98	
09-0ct	02:00	03:00	2.954	0.107	0.99	
09-0ct	03:00	04:00	2.677	0.110	0.98	
09-0ct	04:00	05:00	2.239	0.091	0.98	
09-0ct	05:00	06:00	3.432	0.151	0.98	
09-0ct	06:00	07:00	3.828	0.154	0.98	
09-0ct	07:00	08:00	3.771	0.146	0.98	CALIBRATIONS AND RE-ALIGNMENT
09-0ct	08:00	09:00	7 040			07:31 - 08:43
09-Oct 09-Oct	09:00	10:00	7.946	0.726	0.92	
09-0ct	10:00 11:00	11:00	15.116	0.898	0.97	
09-00t	12:00	12:00 13:00	14.710 15.341	0.809	0.97	
09-0ct	13:00	14:00	16.173	0.819 0.837	0.97 0.97	
09-0ct	14:00	15:00	17.764	0.955	0.97	
09-0ct	15:00	16:00	19.448	0.919	0.98	
09-0ct	16:00	17:00	18.148	0.704	0.98	
09-0ct	17:00	18:00	16.546	0.739	0.98	
09-0ct	18:00	19:00	8.819	0.755	0.96	•
09-0ct	19:00	20:00	5.036	0.299		CALIBRATIONS 19:53 - 20:33
09-0ct	20:00	21:00	4.572	0.217	0.98	
09-0ct	21:00	22:00	3.108	0.215	0.95	
09-0ct	22:00	23:00	4.859	0.304	0.96	
09-0ct	23:00	24:00	6.778	0.156	0.99	
			2	250	2.00	

LOCATION: AZUSA SCAQMD AIR MONITORING STATION
INSTRUMENT: TDLAS

SPECIES: HN03 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE DD-MMM-YY	START TIME PDT	END TIME PDT	MIXING RATIO (PPBV)	95% LIMIT (PPBV)	CORR.	COMMENTS
=======================================					=======	=======================================
10-0ct	00:00	01:00	4.832	0.272	0.97	
10-0ct	01:00	02:00	0.003	0.179	0.00	
10-0ct	02:00	03:00	6.102	0.232	0.98	
10-0ct	03:00	. 04:00	6.845	0.258	0.98	
10-0ct	04:00	05:00	6.586	0.334	0.97	
10-0ct	05:00	06:00	4.872	0.259	0.97	
10-0ct	06:00	07:00	5.915	0.250	0.98	
10-0ct	07:00	08:00				RE-ALIGN OPTICS
10-0ct	08:00	09:00				CALIBRATIONS 08:08 - 09:16
10-0ct	09:00	10:00	1.626	0.243	0.82	
10-0ct	10:00	11:00	9.581	0.336	0.99	
10-0ct	11:00	12:00	13.903	0.322	0.99	
10-0ct	12:00	13:00	16.501	0.504	0.99	
10-0ct	13:00	14:00	16.709	0.801	0.98	
10-0ct	14:00	15:00	16.581	0.493	0.99	
10-0ct	15:00	16:00	17.597	0.534	0.99	
10-0ct	16:00	17:00	12.332	0.298	0.99	
10-0ct	17:00	18:00	11.509	0.227	1.00	
10-0ct	18:00	19:00	11.058	0.295	0.99	
10-0ct	19:00	20:00	5.873	0.176	0.99	
10-0ct	20:00	21:00	7.030	0.230	0.99	
10-0ct	21:00	22:00	4.647	0.130	0.99	CALIBRATION 21:30 - 21:39
10-0ct	22:00	23:00	3.202	0.215	0.95	
10-0ct	23:00	24:00	2.842	0.165	0.96	
11-0ct	00:00	01:00	2.782	0.284	0.86	
11-0ct	01:00	02:00	2.967	0.275	0.88	
11-0ct	02:00	03:00	3.962	0.294	0.92	
11-0ct	03:00	04:00	2.092	0.205	0.87	
11-0ct	04:00	05:00	0.530	0.207	0.41	
11-0ct	05:00	06:00	-0.234	0.330	-0.12	
11-0ct	06:00	07:00	2.359	0.234	0.92	
11-0ct	07:00	08:00	3.611	0.279	0.95	
11-0ct	08:00	09:00	1.824	0.412		CALIBRATION 08:57 - 09:07
11-0ct	09:00	10:00	3.003	0.137	0.98	
11-0ct	10:00	11:00	4.145	0.118	0.99	
11-0ct	11:00	12:00	1.765	0.186	0.90	
11-0ct	12:00	13:00	3.437	0.111	0.99	
11-0ct	13:00	14:00	7.839	0.547	0.95	
11-0ct	14:00	15:00	8.051	0.448	0.97	
11-0ct	15:00	16:00	4.818	0.140	0.99	
11-0ct	16:00	17:00	6.610	0.477	0.95	
11-0ct	17:00	18:00	8.715	0.496	0.97	041 1004 100 40 55 10 10
11-0ct	18:00	19:00	6.321	0.330		CALIBRATION 18:58 - 19:09
11-0ct 11-0ct	19:00	20:00	2.342	0.169	0.95	
11-0ct	20:00	21:00	3.965	0.407	0.90	
11-0ct	21:00 22:00	22:00 23:00	2.017 3.176	0.242	0.87	
11-0ct	23:00	24:00	2.703	0.236	0.95	
11-00L	23:00	24:00	2.703	0.181	0.96	

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS
SPECIES: HN03 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

	DATE DD-MMM-YY	START TIME	END Time	MIXING RATIO	95% LIMIT	CORR.	COMMENTS
		PDT	PDT	(PPBV)	(PPBV)		
٠	12 0-4						=======================================
	12-0ct 12-0ct	00:00	01:00	2.600	0.079	0.99	
	12-0ct	01:00	02:00	-0.064	0.086	-0.16	
	12-0ct	02:00 03:00	03:00	0.469	0.160	0.54	
	12-0ct	04:00	04:00	0.566	0.175	0.57	
	12-0ct	05:00	05:00 06:00	-0.187	0.350	-0.11	
	12-0ct	06:00	07:00	-0.409 1.567	0.187 0.140	-0.43	CALIDRATION OF THE T
	12-0ct	07:00	08:00	2.942	0.140	0.92	CALIBRATION 08:33 - 08:50
	12-0ct	08:00	09:00	1.870	0.133	0.98	
	12-0ct	09:00	10:00	3.284	0.176	0.99	
	12-0ct	10:00	11:00	4.386	0.079		
	12-0ct	11:00	12:00	9.982	0.290	1.00	041 7004 7700 44 44
	12-0ct	12:00	13:00	14.410	0.290		CALIBRATION 11:33 - 11:40
	12-0ct	13:00	14:00	11.451	0.208	1.00	
	12-0ct	14:00	15:00	13.614	0.169	0.99	
	12-0ct	15:00	16:00	6.362	0.151	1.00	
	12-0ct	16:00	17:00	6.549		0.99	
	12-0ct	17:00	18:00	3.039	0.187 0.234	0.99	
	12-0ct	18:00	19:00	3.107	0.234	0.92	041700177011 40 40 40
	12-0ct	19:00	20:00	3.814	0.110		CALIBRATION 18:36 - 18:56
	12-0ct	20:00	21:00	3.135	0.073	1.00	CLEAN INLET PLUMBING
	12-0ct	21:00	22:00	3.714	0.102	0.99	CALIBRATION 20:13 - 20:24
	12-0ct	22:00	23:00	-0.750	0.127	0.99	
	12-0ct	23:00	24:00	-0.276	0.439	-0.45	
	13-0ct	00:00	01:00	-0.135	0.439	-0.14	ETALON MOTOR ON CHARLE
	13-0ct	01:00	02:00	-0.135	0.122		ETALON NOISE ON SYSTEM
	13-0ct	02:00	03:00	-0.135	0.122	-0.23	AVERAGE 00:00 - 09:00
	13-0ct	03:00	04:00	-0.135	0.122	-0.23	
	13-0ct	04:00	05:00	-0.135	0.122	-0.23	
	13-0ct	05:00	06:00	-0.135	0.122	-0.23	
	13-0ct	06:00	07:00	-0.135	0.122	-0.23	
	13-0ct	07:00	08:00	~0.135	0.122	-0.23	
	13-0ct	08:00	09:00	-0.135	0.122		CALIBRATION 08:37 - 08:48
	13-0ct	09:00	10:00	-0.149	0.248	-0.23	CALIBRATION 08:37 - 08:48 CALIBRATION 08:51 - 09:27
	13-0ct	10:00	11:00	0.612	0.244	0.18	BACKGROUND EVERY 10 MIN
	13-0ct	11:00	12:00	1.167	0.257	0.40	TO IMPROVE NIGHTTIME DATA
	13-0ct	12:00	13:00	2.921	0.147	0.97	THE DATA
	13-0ct	13:00	14:00	4.533	0.267	0.96	
	13-0ct	14:00	15:00	5.587	0.302	0.97	
	13-0ct	15:00	16:00	8.486	0.414	0.98	
	13-0ct	16:00	17:00	11.436	0.463	0.98	
	13-0ct	17:00	18:00	8.807	0.407	0.98	
	13-0ct	18:00	19:00	3.271	0.228	0.95	ť
	13-0ct	19:00	20:00	0.692	0.035	0.97	
	13-0ct	20:00	21:00	0.585	0.037		CALIBRATION 20:39 - 20:47
	13-0ct	21:00	22:00	0.113	0.055	0.41	20:47
	13-0ct	22:00	23:00	-0.046	0.015	-0.55	
	13-0ct	23:00	24:00	0.044	0.044	0.21	
						•	

LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS

SPECIES: HN03 - 1 HOUR AVERAGES

PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

PDT	DATE DD-MMM-YY	START TIME	END TIME	MIXING RATIO	95% Limit	CORR.	COMMENTS
14-Oct 00:00 01:00 0.170 0.043 0.85 14-Oct 01:00 02:00 0.411 0.062 0.82 14-Oct 02:00 03:00 0.386 0.048 0.87 14-Oct 02:00 03:00 0.202 0.056 0.61 14-Oct 03:00 0.500 0.202 0.056 0.61 14-Oct 05:00 06:00 0.372 0.057 0.82 14-Oct 05:00 08:00 0.372 0.057 0.82 14-Oct 07:00 08:00 0.095 0.117 0.17 14-Oct 08:00 09:00 0.355 0.111 0.57 CALIBRATION 08:33 - 08:41 14-Oct 09:00 10:00 0.410 0.184 0.43 14-Oct 10:00 11:00 1.045 0.087 0.93 14-Oct 11:00 12:00 1.666 0.077 0.98 14-Oct 12:00 13:00 4.530 0.213 0.98 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 14:00 15:00 10.950 0.252 0.99 14-Oct 15:00 16:00 15.818 0.318 1.00 14-Oct 17:00 18:00 6.119 0.245 0.98 14-Oct 19:00 17:00 1.0304 0.183 1.00 14-Oct 19:00 20:00 1.009 0.055 0.99 14-Oct 19:00 20:00 1.009 0.057 0.99 14-Oct 21:00 18:00 6.119 0.245 0.98 14-Oct 21:00 20:00 1.009 0.057 0.99 14-Oct 21:00 0.957 0.039 0.99 14-Oct 19:00 20:00 1.009 0.057 0.99 14-Oct 19:00 20:00 1.009 0.057 0.99 14-Oct 21:00 0.957 0.039 0.99 14-Oct 21:00 0.957 0.039 0.99 14-Oct 21:00 0.087 0.099 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 22:00 23:00 0.957 0.039 0.98 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.99 15-Oct 00:00 01:00 0.683 0.037 0.97 15-Oct 00:00 01:00 0.887 0.039 0.98 15-Oct 00:00 07:00 0.887 0.035 0.98 15-Oct 00:00 07:00 0.887 0.035 0.98 15-Oct 00:00 07:00 0.887 0.035 0.98 15-Oct 00:00 07:00 0.880 0.026 0.99 15-Oct 10:00 00:00 1.467 0.032 0.99 15-Oct 11:00 12:00 5.285 0.049 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 11:00 12:00 5.584 0.215 0.98 15-Oct 11:00 12:00 5.584 0.215 0.98 15-Oct 11:00 10:00 1.487 0.032 0.99 15-Oct 11:00 12:00 5.584 0.041 1.00 15-Oct 11:00 12:00 5.584 0.011 0.99 15-Oct 11:00 10:00 1.487 0.02							
14-Oct 01:00 02:00 0.411 0.062 0.82 14-Oct 02:00 03:00 0.386 0.048 0.87 14-Oct 02:00 0,04:00 0.202 0.056 0.61 14-Oct 04:00 05:00 0.255 0.061 0.67 14-Oct 06:00 07:00 -0.027 0.105 -0.08 14-Oct 06:00 07:00 -0.027 0.105 -0.08 14-Oct 07:00 08:00 0.955 0.117 0.17 14-Oct 09:00 10:00 0.355 0.111 0.57 CALIBRATION 08:33 - 08:41 14-Oct 09:00 10:00 0.410 0.084 0.43 14-Oct 10:00 11:00 1.045 0.087 0.93 14-Oct 11:00 12:00 1.666 0.077 0.98 14-Oct 11:00 12:00 1.666 0.077 0.98 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 16:00 15:00 10.950 0.252 0.99 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 16:00 17:00 10.304 0.183 1.00 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 19:00 20:00 1.090 0.052 0.99 14-Oct 19:00 20:00 1.009 0.052 0.99 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 21:00 22:00 0.822 0.43 0.99 14-Oct 21:00 0.000 0.0057 0.039 0.99 14-Oct 21:00 0.0057 0.039 0.99 14-Oct 21:00 0.0057 0.039 0.99 14-Oct 21:00 0.0057 0.039 0.99 14-Oct 23:00 24:00 0.857 0.039 0.99 14-Oct 23:00 24:00 0.859 0.069 0.75 15-Oct 00:00 01:00 0.683 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.99 15-Oct 01:00 02:00 0.887 0.035 0.99 15-Oct 01:00 07:00 2.285 0.049 1.00 15-Oct 01:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 01:00 19:00 3.50 0.090 15-Oct 01:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 01:00 19:00 3.00 0.92 15-Oct 11:00 11:00 2.210 0.0867 0.035 0.99 15-Oct 11:00 11:00 2.00 0.0867 0.035 0.99 15-Oct 11:00 11:00 5.216 0.043 1.00 15-Oct 11:00 11:00 2.00 0.0867 0.035 0.99 15-Oct 11:00 0.00 0.00 0.00 0.00 0.00 0.00 0.0							=======================================
14-Oct 03:00 03:00 0.386 0.048 0.87 14-Oct 03:00 0.40:00 0.202 0.056 0.61 14-Oct 04:00 05:00 0.205 0.061 0.67 14-Oct 05:00 06:00 0.372 0.057 0.82 14-Oct 07:00 08:00 0.372 0.057 0.82 14-Oct 07:00 08:00 0.095 0.117 0.17 14-Oct 08:00 09:00 0.355 0.111 0.57 CALIBRATION 08:33 - 08:41 14-Oct 08:00 09:00 1.000 0.410 0.184 0.43 14-Oct 10:00 11:00 1.045 0.087 0.93 14-Oct 10:00 13:00 1.045 0.087 0.93 14-Oct 12:00 13:00 4.530 0.213 0.98 14-Oct 12:00 13:00 4.530 0.213 0.98 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 17:00 18:00 6.119 0.245 0.98 14-Oct 18:00 19:00 3.353 0.109 0.99 14-Oct 18:00 19:00 3.353 0.109 0.99 14-Oct 18:00 19:00 3.034 0.183 1.00 14-Oct 18:00 19:00 3.004 0.183 1.00 14-Oct 18:00 19:00 3.004 0.183 1.00 14-Oct 18:00 0.957 0.099 0.99 14-Oct 18:00 0.957 0.099 0.99 14-Oct 18:00 0.957 0.099 0.99 14-Oct 19:00 0.000 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 20:00 21:00 0.957 0.039 0.99 14-Oct 20:00 0.087 0.099 0.75 15-Oct 01:00 0.000 0.887 0.093 0.99 15-Oct 01:00 0.000 0.887 0.093 0.99 15-Oct 01:00 0.000 0.887 0.093 0.99 15-Oct 01:00 0.000 0.000 0.997 0.099 15-Oct 01:00 0.000 0.000 0.997 0.046 0.97 15-Oct 01:00 0.000 0.000 0.900 0.000 0.99 15-Oct 11:00 11:00 0.063 0.037 0.97 15-Oct 01:00 0.000 0.000 0.900 0.000 0.000 0.900 0.							
14-Oct 03:00							
14-Oct							
14-Oct 05:00 06:00 0.372 0.057 0.82 14-Oct 07:00 08:00 0.905 0.117 0.17 14-Oct 08:00 09:00 0.955 0.117 0.17 14-Oct 08:00 09:00 0.355 0.111 0.57 CALIBRATION 08:33 - 08:41 14-Oct 10:00 11:00 1.045 0.087 0.93 14-Oct 11:00 12:00 1.666 0.077 0.98 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 16:00 17:00 10.304 0.183 1.00 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 21:00 22:00 0.782 0.043 0.98 14-Oct 21:00 22:00 0.987 0.039 0.98 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 03:00 04:00 0.927 0.049 1.00 15-Oct 07:00 08:00 1.090 0.052 0.99 15-Oct 07:00 08:00 1.090 0.052 0.99 15-Oct 08:00 09:00 1.090 0.026 0.99 15-Oct 10:00 11:00 1.000 0.026 0.99 15-Oct 11:00 12:00 1.000 0.026 0.99 15-Oct 11:00 12:00 1.000 0.026 0.99 15-Oct 11:00 12:00 5.216 0.049 1.000 15-Oct 11:00 12:00 0.800 1.090 0.026 0.99 15-Oct 11:00 12:00 0.501 1.511 0.084 0.98 15-Oct 11:00 12:00 0.501 1.511 0.084 0.98 15-Oct 11:00 12:00 0.501 1.011 0.084 0.98 15-Oct 11:00 12:00 0.501 1.000 0.026 0.99 15-Oct 11:00 12:00 0.501 1.000 0.001 0.001 1.000 0.001			•				
14-Oct 06:00 07:00 -0.027 0.105 -0.08 14-Oct 07:00 08:00 0.095 0.117 0.17 14-Oct 08:00 09:00 0.355 0.111 0.57 14-Oct 09:00 10:00 0.410 0.184 0.43 14-Oct 10:00 11:00 1.045 0.087 0.93 14-Oct 11:00 12:00 1.666 0.077 0.98 14-Oct 12:00 13:00 4.530 0.213 0.98 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 14:00 15:00 10.950 0.252 0.99 14-Oct 15:00 16:00 15.818 0.318 1.00 14-Oct 17:00 18:00 15.818 0.318 1.00 14-Oct 17:00 18:00 6.119 0.245 0.98 14-Oct 19:00 20:00 1.009 0.052 0.99 14-Oct 19:00 20:00 1.009 0.052 0.99 14-Oct 19:00 20:00 1.009 0.052 0.97 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 21:00 22:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.957 0.039 0.99 14-Oct 20:00 21:00 0.957 0.039 0.98 15-Oct 01:00 02:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.683 0.037 0.97 15-Oct 01:00 02:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 08:00 09:00 1.316 0.025 1.00 15-Oct 08:00 09:00 1.316 0.025 1.00 15-Oct 08:00 09:00 1.316 0.025 1.00 15-Oct 11:00 12:00 0.2285 0.049 1.00 15-Oct 11:00 12:00 0.026 0.99 15-Oct 11:00 12:00 0.061 0.99 15-Oct 11:00 12:00 0.001 1.000 0.98 15-Oct 11:00 12:00 0.001 1.000 0.98 15-Oct 11:00 12:00 0.001 0.001 0.99 15-Oct 11:00 12:00 0.001 0.001 0.99 15-Oct 11:00 10:00 0.001 0.001 0.99 15-Oct 11:00 0.001 0.001 0.001 0.001 0.001 0.99 15-Oct							
14-Oct 07:00 08:00 09:00 0.095 0.117 0.17 14-Oct 08:00 09:00 10:00 0.355 0.111 0.57 CALIBRATION 08:33 - 08:41 14-Oct 19:00 11:00 1.045 0.087 0.93 14-Oct 11:00 12:00 1.666 0.077 0.98 14-Oct 11:00 12:00 1.666 0.077 0.98 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 16:00 17:00 10.304 0.183 1.00 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 10:00 02:00 0.887 0.035 0.98 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 10:00 02:00 0.880 0.006 0.99 15-Oct 10:00 02:00 0.880 0.006 0.99 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 10:00 01:00 1.467 0.032 0.99 15-Oct 10:00 01:00 1.467 0.032 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 15:00 16:00 17:00 2.010 0.061 0.99 15-Oct 11:00 12:00 5.266 0.043 1.00 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.387 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42							
14-Oct 09:00 09:00 10:00 0.355 0.111 0.57 CALIBRATION 08:33 - 08:41 14-Oct 10:00 11:00 1.410 0.184 0.43   14-Oct 10:00 11:00 1.045 0.087 0.93   14-Oct 11:00 12:00 1.666 0.077 0.98   14-Oct 12:00 13:00 4.530 0.213 0.98   14-Oct 13:00 14:00 7.317 0.129 1.00   14-Oct 13:00 16:00 15.818 0.316 1.00   14-Oct 15:00 16:00 15.818 0.316 1.00   14-Oct 17:00 18:00 6.119 0.245 0.98   14-Oct 17:00 18:00 6.119 0.245 0.98   14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23   14-Oct 20:00 21:00 0.957 0.039 0.98   14-Oct 20:00 21:00 0.957 0.039 0.98   14-Oct 22:00 23:00 0.917 0.029 0.99   14-Oct 22:00 23:00 0.917 0.029 0.99   14-Oct 22:00 23:00 0.917 0.029 0.99   14-Oct 23:00 24:00 0.359 0.069 0.75   15-Oct 00:00 01:00 0.663 0.037 0.97   15-Oct 01:00 02:00 0.663 0.037 0.97   15-Oct 03:00 04:00 0.927 0.046 0.98   15-Oct 05:00 06:00 2.330 0.040 1.00   15-Oct 05:00 06:00 2.330 0.040 1.00   15-Oct 05:00 06:00 2.330 0.040 1.00   15-Oct 06:00 07:00 2.285 0.049 1.00   15-Oct 07:00 08:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38   15-Oct 10:00 10:00 1.467 0.032 0.99   15-Oct 10:00 10:00 1.467 0.032 0.99   15-Oct 11:00 12:00 5.216 0.061 0.99   15-Oct 11:00 12:00 5.216 0.061 0.99   15-Oct 11:00 11:00 2.210 0.061 0.99   15-Oct 11:00 11:00 0.000							
14-Oct							CALIBRATION OF 22 - 00.41
14-Oct 10:00 11:00 1.045 0.087 0.93 14-Oct 11:00 12:00 1.666 0.077 0.98 14-Oct 12:00 13:00 4.530 0.213 0.98 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 15:00 16:00 15:818 0.316 1.00 14-Oct 16:00 17:00 10.304 0.183 1.00 14-Oct 17:00 18:00 6.119 0.245 0.98 14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 02:00 03:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 04:00 05:00 1.511 0.064 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 11:00 01:00 0.00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 15:00 16:00 4.740 0.074 1.00 15-Oct 15:00 16:00 4.740 0.074 1.00 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42							CALIBRATION 08.33 - 08:41
14-Oct 11:00 12:00 1.666 0.077 0.98 14-Oct 12:00 13:00 4.530 0.213 0.98 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 14:00 15:00 10.950 0.252 0.99 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 16:00 17:00 10.304 0.183 1.00 14-Oct 17:00 18:00 6.119 0.245 0.98 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 01:00 02:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.687 0.035 0.98 15-Oct 02:00 03:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 04:00 05:00 1.511 0.084 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 12:00 5.216 0.025 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.049 1.00 15-Oct 11:00 12:00 5.216 0.049 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 15:0ct 15:00 16:00 4.184 0.190 0.98 15-Oct 15:0ct 15:00 16:00 4.740 0.074 1.00 15-Oct 15:0ct 15:00 16:00 4.089 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42							
14-Oct 12:00 13:00 4.530 0.213 0.98 14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 14:00 15:00 10.950 0.252 0.99 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 16:00 17:00 10.304 0.183 1.00 14-Oct 18:00 19:00 3.535 0.109 0.98 14-Oct 19:00 20:00 1.009 0.052 0.97 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 22:00 0.350 0.917 0.029 0.99 14-Oct 22:00 0.887 0.035 0.98 15-Oct 01:00 02:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 04:00 05:00 1.511 0.084 0.98 15-Oct 05:00 06:00 0.927 0.046 0.97 15-Oct 05:00 06:00 0.927 0.046 0.97 15-Oct 05:00 06:00 0.930 0.0682 0.071 0.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 08:00 07:00 2.285 0.049 1.00 15-Oct 08:00 07:00 2.285 0.049 1.00 15-Oct 08:00 07:00 2.285 0.049 1.00 15-Oct 10:00 11:00 0.201 0.061 0.09 15-Oct 10:00 11:00 2.210 0.061 0.09 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.09 15-Oct 18:00 17:00 3.898 0.131 0.09 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42							
14-Oct 13:00 14:00 7.317 0.129 1.00 14-Oct 14:00 15:00 10.950 0.252 0.99 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 15:00 16:00 17:00 10.304 0.183 1.00 14-Oct 17:00 18:00 6.119 0.245 0.98 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 01:00 00:00 0.663 0.037 0.97 15-Oct 01:00 00:00 0.663 0.037 0.97 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 04:00 05:00 1.511 0.084 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 11:00 12:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.387 0.242 0.99 15-Oct 18:00 17:00 3.898 0.131 0.99 15-Oct 18:00 17:00 3.898 0.131 0.99 15-Oct 18:00 17:00 3.898 0.131 0.99 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42							
14-Oct 14:00 15:00 10.950 0.252 0.99 14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 16:00 17:00 10.304 0.183 1.00 14-Oct 17:00 18:00 6.119 0.245 0.98 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 22:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 02:00 03:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 04:00 05:00 1.511 0.064 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 09:00 11:00 2.210 0.061 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 11:00 12:00 5.981 0.139 0.99 15-Oct 11:00 12:00 5.981 0.139 0.99 15-Oct 11:00 15:00 5.564 0.215 0.98 15-Oct 11:00 15:00 5.564 0.215 0.98 15-Oct 11:00 16:00 4.184 0.190 0.99 15-Oct 11:00 18:00 4.387 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 18:00 19:00 2.099 0.104 0.89							
14-Oct 15:00 16:00 15.818 0.316 1.00 14-Oct 16:00 17:00 10.304 0.183 1.00 14-Oct 17:00 18:00 6.119 0.245 0.98 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 02:00 03:00 0.682 0.071 0.90 15-Oct 04:00 05:00 1.511 0.084 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 12:00 5.216 0.043 1.00 15-Oct 11:00 12:00 5.564 0.215 0.99 15-Oct 11:00 15:00 5.564 0.215 0.99 15-Oct 14:00 15:00 5.564 0.215 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.387 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42							
14-Oct 16:00 17:00 10:304 0.183 1.00 14-Oct 17:00 18:00 6.119 0.245 0.98 14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 02:00 03:00 0.662 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 04:00 05:00 1.511 0.064 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 09:00 10:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.03 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 17:00 18:00 4.387 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89	14-0ct						
14-Oct 18:00 19:00 3.535 0.109 0.99 14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.089 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 00:00 03:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 06:00 07:00 08:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 12:00 5.216 0.061 0.99 15-Oct 11:00 12:00 5.216 0.061 0.99 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.69	14-0ct	16:00	17:00	10.304			
14-Oct 19:00 20:00 1.009 0.052 0.97 CALIBRATION 19:13 - 19:23 14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 15:00 16:00 5.981 0.139 0.99 15-Oct 15:00 16:00 4.780 0.074 1.00 15-Oct 15:00 16:00 4.780 0.074 1.00 15-Oct 15:00 16:00 4.784 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89	14-0ct	17:00	18:00	6.119	0.245	0.98	
14-Oct 20:00 21:00 0.957 0.039 0.98 14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 21:00 22:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.990 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.387 0.242 0.97 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89	14-0ct	18:00	19:00	3.535	0.109	0.99	
14-Oct 21:00 22:00 0.782 0.043 0.97 14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 02:00 03:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 04:00 05:00 1.511 0.064 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89	14-0ct	19:00	20:00	1.009	0.052	0.97	CALIBRATION 19:13 - 19:23
14-Oct 22:00 23:00 0.917 0.029 0.99 14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 02:00 03:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89	14-0ct	20:00	21:00	0.957	0.039	0.98	
14-Oct 23:00 24:00 0.359 0.069 0.75 15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 02:00 03:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 04:00 05:00 1.511 0.064 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89		21:00	22:00	0.782	0.043	0.97	
15-Oct 00:00 01:00 0.663 0.037 0.97 15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 02:00 03:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 03:00 05:00 1.511 0.064 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89		22:00	23:00	0.917	0.029	0.99	
15-Oct 01:00 02:00 0.887 0.035 0.98 15-Oct 02:00 03:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 03:00 05:00 1.511 0.064 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89					0.069		
15-Oct 02:00 03:00 0.682 0.071 0.90 15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 04:00 05:00 1.511 0.084 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89							
15-Oct 03:00 04:00 0.927 0.046 0.97 15-Oct 04:00 05:00 1.511 0.084 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89							
15-Oct 04:00 05:00 1.511 0.084 0.98 15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89							
15-Oct 05:00 06:00 2.330 0.040 1.00 15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89							
15-Oct 06:00 07:00 2.285 0.049 1.00 15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 19:00 20:00 0.929 0.104 0.89							
15-Oct 07:00 08:00 1.090 0.026 0.99 15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							
15-Oct 08:00 09:00 1.316 0.025 1.00 CALIBRATION 08:28 - 08:38 15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							
15-Oct 09:00 10:00 1.467 0.032 0.99 15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							CALEBRATION OR OR OR OR
15-Oct 10:00 11:00 2.210 0.061 0.99 15-Oct 11:00 12:00 5.216 0.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 15:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							CALIBRATION 08:28 - 08:38
15-Oct 11:00 12:00 5.216 Q.043 1.00 15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							
15-Oct 12:00 13:00 4.740 0.074 1.00 15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							
15-Oct 13:00 14:00 5.981 0.139 0.99 15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							
15-Oct 14:00 15:00 5.564 0.215 0.98 15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							
15-Oct 15:00 16:00 4.184 0.190 0.98 15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							
15-Oct 16:00 17:00 3.898 0.131 0.99 15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							
15-Oct 17:00 18:00 4.367 0.242 0.97 15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							
15-Oct 18:00 19:00 2.198 0.041 1.00 CALIBRATION 18:33 - 18:42 15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92							
15-Oct 19:00 20:00 0.929 0.104 0.89 15-Oct 20:00 21:00 0.741 0.067 0.92	15-0ct						CALIBRATION 18:33 - 18:42
	15-0ct	19:00	20:00	0.929	0.104		
15-Oct 21:00 22:00 0.728 0.039 0.97	15-0ct	20:00	21:00	0.741	0.067	0.92	
		21:00	22:00	0.728	0.039	0.97	
15-Oct 22:00 23:00 0.178 0.029 0.80			23:00	0.178	0.029	0.80	
15-Oct 23:00 24:00 0.328 0.035 0.90	15-Oct	23:00	24:00	0.328	0.035	0.90	

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS
SPECIES: HNO3 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE DD-MMM~YY	START Time	END Time	MIXING RATIO	95% LIMIT	CORR.	COMMENTS
	PDT	PDT	(PPBV)	(PPBV)		
=======================================						=======================================
16-0ct	00:00	01:00	0.266	0.051	0.75	
16-0ct	01:00	02:00	0.280	0.045	0.80	
16-0ct	02:00	03:00	0.319	0.053	0.79	
16-0ct	03:00	04:00	0.216	0.092	0.45	
16-0ct	04:00	05:00	0.578	0.035	0.96	
16-0ct	05:00	06:00	0.295	0.257	0.24	
16-0ct	06:00	07:00	0.275	0.037	0.85	
16-0ct	07:00	08:00	0.463	0.090	0.74	
16-0ct	08:00	09:00	0.481	0.098	0.73	CALIBRATION 08:56 - 09:04
16-0ct	09:00	10:00	0.465	0.038	0.94	
16~0ct	10:00	11:00	0.427	0.044	0.90	
16-0ct	11:00	12:00	1.244	0.068	0.97	
16-0ct	12:00	13:00	1.829	0.048	0.99	
16-0ct	13:00	14:00	2.716	0.050	1.00	
16-0ct	14:00	15:00	2.077	0.046	0.99	
16-0ct	15:00	16:00	1.352	0.071	0.97	
16-0ct	16:00	17:00	1.125	0.039	0.99	
16-0ct	17:00	18:00	1.126	0.032	0.99	
16-0ct	18:00	19:00	0.848	0.022	0.99	
16-0ct	19:00	20:00	0.874	0.041	0.98	
16-0ct	20:00	21:00	0.627	0.033	0.97	CALIBRATION 20:30 - 20:40
16-0ct	21:00	22:00	0.133	0.073	0.37	
16-0ct	22:00	23:00	0.320	0.061	0.75	
16-0ct	23:00	24:00	0.335	0.038	0.88	
17-0ct	00:00	01:00	0.202	0.049	0.66	
17-0ct	01:00	02:00	0.488	0.091	0.76	
17-0ct	02:00	03:00	0.553	0.051	0.92	
17-0ct	03:00	04:00	0.640	0.063	0.91	
17-0ct	04:00	05:00	0.332	0.082	0.66	
17-0ct	05:00	06:00	0.760	0.152	0.74	
17-0ct	06:00	07:00	0.208	0.111	0.38	
17-0ct	07:00	08:00	0.572	0.058	0.91	
17-0ct	08:00	09:00	0.642	0.100	0.81	CALIBRATION 08:46 - 08:45
17-0ct	09:00	10:00	1.428	0.060	0.98	
17-0ct	10:00	11:00	1.860	0.059	0.99	
17-0ct	11:00	12:00	3.637	0.101	0.99	
17-0ct	12:00	13:00	6.197	0.229	0.99	
17-0ct	13:00	14:00	5.329	0.137	0.99	
17-0ct	14:00	15:00	6.529	0.160	0.99	
17-0ct 17-0ct	15:00	16:00	5.589	0.172	0.99	
17-0ct	16:00	17:00	4.936	0.214	0.98	
17-0ct	17:00	18:00	3.902	0.119	0.99	t .
17-0ct	18:00 19:00	19:00	1.510	0.039	0.99	
17-0ct	20:00	20:00	1.299	0.041	0.99	
17-0ct	21:00	21:00	1.116	0.043	0.98	04110017100 04 05 05
17-0ct	22:00	22:00	0.981	0.034	0.99	CALIBRATION 21:25 - 21:34
17-0ct	22:00	23:00	0.298	0.083	0.61	
17-001	23:00	24:00	0.345	0.058	0.79	

LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS

SPECIES: HN03 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE	START	END	MININO	0.5%	0000	0011151150
DD-MMM-YY	TIME	END Time	MIXING RATIO	95%	CORR.	COMMENTS
DD-MMM-11	PDT	PDT	(PPBV)	LIMIT (PPBV)	COEFF.	
===========						
18-0ct	00:00	01:00	0.352	0.026	0.95	
18-0ct	01:00	02:00	0.347	0.068	0.74	
18-0ct	02:00	03:00	0.679	0.165	0.66	
18-0ct	03:00	, 04:00	0.012	0.084	0.03	
18-0ct	04:00	05:00	0.820	0.099	0.87	
18-0ct	05:00	06:00	0.118	0.053	0.43	
18-0ct	06:00	07:00	0.353	0.075	0.71	
18-0ct	07:00	08:00	0.288	0.145	0.40	
18-0ct	08:00	09:00	0.447	0.104	0.68	CALIBRATIONS 08:42 - 08:53
18-0ct	09:00	10:00	0.432	0.093	0.71	
18-0ct	10:00	11:00	1.502	0.042	0.99	
18-0ct	11:00	12:00	2.580	0.047	1.00	
18-0ct	12:00	13:00	3.985	0.107	0.99	
18-0ct	13:00	14:00	4.265	0.077	1.00	
18-0ct	14:00	15:00	6.743	0.164	0.99	
18-0ct	15:00	16:00	7.144	0.242	0.99	
18-0ct	16:00	17:00	4.720	0.324	0.95	
18-0ct	17:00	18:00	3.431	0.335	0.91	
18-0ct	18:00	19:00	1.311	0.047	0.99	
18-0ct	19:00	20:00	1.005	0.039	0.98	
18-0ct	20:00	21:00	0.926	0.028	0.99	
18-0ct	21:00	22:00	1.321	0.033	0.99	CALIBRATIONS 21:25 - 21:35
18-0ct	22:00	23:00	0.902	0.068	0.94	
18-0ct	23:00	24:00	0.238	Ò.047	0.74	
19-0ct	00:00	01:00	0.416	0.059	0.84	
19-0ct	01:00	02:00	0.730	0.058	0.94	
19-0ct	02:00	03:00	0.266	0.053	0.74	
19-0ct	03:00	04:00	0.510	0.040	0.94	
19-0ct	04:00	05:00	0.514	0.049	0.92	
19-0ct	05:00	06:00	0.236	0.097	0.47	
19-0ct	06:00	07:00	-0.114	0.095	-0.25	
19-0ct	07:00	08:00	-0.076	0.139	-0.12	
19-0ct	08:00	09:00	-0.134	0.185	-0.16	
19-0ct	09:00	10:00	1.651	0.094		CALIBRATION 09:09 - 09:21
19-0ct	10:00	11:00	3.937	0.227		NO TEFLON FILTER IN LINE
19-0ct	11:00	12:00	7.078	0.242		SAMPLING AT VAN ROOF LEVEL
19-0ct 19-0ct	12:00	13:00	7.587	0.184	0.99	
19-0ct	13:00 14:00	14:00	6.374	0.050	1.00	
19-0ct	15:00	15:00 16:00	6.245	0.109	1.00	
19-0ct	18:00	17:00	6.553 7.010	0.149	0.99	
19-0ct	17:00	18:00	6.158	0.192	0.99	
19-0ct	18:00	19:00	4.556	0.145 0.262	0.99 0.97	
19-0ct	19:00	20:00	2.086	0.202	0.98	
19-0ct	20:00	21:00	1.902	0.058	0.98	
19-0ct	21:00	22:00	1.561	0.045		CALIBRATION 20:59 - 21:08
19-0ct	22:00	23:00	2.551	0.057	0.99	ONCIDENTION 20:09 - 21:08
19-0ct	23:00	24:00	1.617	0.075	0.98	

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS

SPECIES: HNO3 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE	START	END	MIXING	95%	CORR.	COMMENTS
DD-MMM-YY	TIME	TIME	RATIO	LIMIT	COEFF.	
	PDT	PDT	(PPBV)	(PPBV)		
						***********
20-0ct	00:00	01:00	1.347	0.069	0.97	
20-0ct	01:00	02:00	1.382	0.058	0.98	
20-0ct	02:00	03:00	0.687	0.049	0.95	
20-0ct	03:00	04:00	0.864	0.025	0.99	
20-0ct	04:00	05:00	0.909	0.039	0.98	
20-0ct	05:00	06:00	0.813	0.085	0.90	
20-0ct	06:00	07:00	1.142	0.038	0.99	
20-0ct 20-0ct	07:00 08:00	08:00	0.384	0.202 0.090	0.38 0.89	
20-00t		09:00 10:00	0.822 2.414	0.059		CALIBRATION 09:01 - 09:18
20-0ct 20-0ct	09:00 10:00		5.215	0.286	0.97	CALIBRATION 09:01 - 09:16
20-001 20-001	11:00	11:00	7.807	0.147	1.00	
20-0ct	12:00	12:00 13:00	8.896	0.147	1.00	•
20-0ct	13:00	14:00	8.795	0.037	1.00	
20-0ct	14:00	15:00	7.921	0.173		BACKGROUND 14:40 - 14:52
20-0ct	15:00	16:00	8.305	0.172	1.00	BACKGROUND 14.40 - 14.52
20-0ct	16:00	17:00	9.633	0.172	1.00	
20-0ct	17:00	18:00	10.020	0.107	0.99	
20-0ct	18:00	19:00	6.309	0.377	0.96	
20-0ct		20:00	5.032	0.214		
20-0ct	19:00 20:00		3.332	0.214	0.98 0.94	
20-00t 20-0ct		21:00				
20-00t 20-0ct	21:00 22:00	22:00	1.203	0.080 0.099	0.96	
20-0ct	23:00	23:00	1.466 1.114	0.099	0.95 0.95	
21-0ct	00:00	24:00	1.229	0.077	1.00	
21-0ct	01:00	01:00 02:00	2.418	0.023	0.99	
21-0ct	02:00					
21-0ct 21-0ct	02:00	03:00 04:00	2.576 2.556	0.067	0.99	
21-0ct	04:00	05:00	1.718	0.041 0.051	1.00 0.99	
21-0ct	05:00	06:00	2.460	0.031	1.00	
21-0ct	06:00	07:00	2.366	0.037	1.00	
21-0ct	07:00	08:00	1.393	0.191	0.85	
21-0ct	08:00	09:00	0.197	0.200	0.21	
21-0ct	09:00	10:00	0.757	0.200	0.21	CALIBRATION 09:11 - 09:22
21-0ct	10:00	11:00				SYSTEM CHECKS 09:00 - 11:14
21-0ct	11:00	12:00	5.547	0.199	0.99	
21-0ct	12:00	13:00	7.804	0.053	1.00	
21-0ct	13:00	14:00	7.860	0.242	0.99	
21-0ct	14:00	15:00	8.206	0.133	1.00	
21-0ct	15:00	16:00	9.115	0.136	1.00	
21-0ct	16:00	17:00	11.470	0.312	0.99	
21-0ct	17:00	18:00	8.388	0.436	0.97	
21-0ct	18:00	19:00	8.239	0.273	0.99	é .
21-0ct	19:00	20:00	5.009	0.534	0.90	
21-0ct	20:00	21:00	1.750	0.334	0.96	
21-0ct	21:00	22:00	0.877	0.110		CALIBRATION 21:40 - 21:50
21-0ct	22:00	23:00	1.232	0.164	0.85	
21-0ct	23:00	24:00	2.778	0.109	0.98	
2. 001	-3.03	_ 4.00	,,0	0.105	0.50	

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS

SPECIES: HN03 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE	START	END	MIXING	95%	CORR.	COMMENTS
DD-MMM-YY	TIME	TIME	RATIO	LIMIT	COEFF.	
	PDT	PDT	(PPBV)	(PPBV)		
22-0ct	00:00	01:00				*********
22-0ct 22-0ct			1.597	0.056	0.99	
	01:00	02:00	1.745	0.092	0.97	
22-0ct	02:00	03:00	2.579	0.133	0.97	
22-0ct	03:00	, 04:00	2.425	0.080	0.99	
22-0ct	04:00	05:00	2.002	0.147	0.95	
22-0ct	05:00	06:00	2.631	0.070	0.99	
22-0ct	06:00	07:00	1.022	0.247	0.67	
22-0ct	07:00	08:00	1.343	0.088	0.96	
22-0ct	08:00	09:00	1.428	0.087		CALIBRATION 08:36 - 08:47
22-0ct	09:00	10:00	2.677	0.085	0.99	
22-0ct	10:00	11:00	6.295	0.105	1.00	
22-0ct	11:00	12:00	7.094	0.256	0.99	
22-0ct	12:00	13:00	5.668	0.174	0.99	
22-0ct	13:00	14:00	2.310	0.279	0.87	
22-0ct	14:00	15:00	3.264	0.388	0.88	
22-0ct	15:00	16:00	3.076	0.245	0.94	
22-0ct	16:00	17:00	7.025	0.395	0.97	
22-0ct	17:00	18:00	9.430	0.272		CALIBRATION 17:16 - 17:27
22-0ct	18:00	19:00	7.808	0.298	0.98	
22-0ct	19:00	20:00	6.859	0.283	0.98	
22-0ct	20:00	21:00	4.923	0.249	0.97	
22-0ct	21:00	22:00	2.589	0.104	0.98	
22-0ct	22:00	23:00	1.351	0.075	0.97	
22-0ct	23:00	24:00	0.229	0.327	0.15	
23-0ct	00:00	01:00	0.387	0.260	0.31	
23-0ct	01:00	02:00	1.038	0.092	0.93	
23-0ct	02:00	03:00	1.797	0.092	0.97	
23-0ct	03:00	04:00	1.494	0.059	0.98	
23-0ct	04:00	05:00	1.652	0.141	0.93	
23-0ct 23-0ct	05:00	06:00	1.466	0.038	0.99	
23-0ct	06:00	07:00	0.670	0.188	0.61	***********
23-0ct	07:00	08:00	1.695	0.145		CALIBRATION 07:12 - 07:23
23-0ct	08:00	09:00	2.326	0.065	0.99	
23-0ct	09:00	10:00	2.564	0.085	0.99	
23-0ct	10:00	11:00	7.052	0.292	0.98	
23-0ct 23-0ct	11:00	12:00	8.118	0.285	0.99	
23-0ct	12:00	13:00	9.742	0.375	0.98	
23-0ct	13:00 14:00	14:00	10.476	0.438		BACKGROUND TEST 13:14 - 13:35
23-0ct	15:00	15:00 16:00	11.737	0.419	0.99	
23-0ct	16:00		13.974	0.440	0.99	
23-0ct	17:00	17:00	13.308	0.534	0.98	
23-0ct 23-0ct	18:00	18:00	10.008	0.411	0.98	
23-0ct	19:00	19:00	6.847	0.275	0.98	
23-0ct 23-0ct	20:00	20:00	5.192	0.208	0.98	
23-0ct	21:00	21:00	3.452	0.131	0.98	CALIFORNIA OF STATE
23-0ct 23-0ct		22:00	1.326	0.078		CALIBRATION 21:05 - 21:19
23-0ct 23-0ct	22:00	23:00	1.211	0.123		BACKGROUND TEST 21:19 - 21:28
23-001	23:00	24:00	1.072	0.073	0.95	

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS
SPECIES: HNO3 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE DD-MMM-YY	START TIME PDT	END TIME PDT	MIXING RATIO (PPBV)	95% LIMIT (PPBV)	CORR.	COMMENTS
	00:00	01:00	0.727	0.135		
24-0ct					0.76	
24-0ct	01:00	02:00	0.395	0.183	0.42	
24-0ct	02:00	03:00	0.505	0.041	0.94	
24-0ct	03:00	04:00	0.510	0.228	0.44	
24-0ct 24-0ct	04:00 05:00	05:00 06:00	0.737 0.231	0.078 0.209	0.90 0.23	
24-0ct	06:00	07:00	0.478	0.081	0.79	
24-0ct	07:00	08:00	0.680	0.112	0.80	
24-0ct	08:00	09:00	0.129	0.172	0.16	
24-0ct	09:00	10:00	0.346	0.159		CALIBRATION 09:01 - 09:12
24-0ct	10:00	11:00	0.510	0.119	0.68	0.01
24-0ct	11:00	12:00	6.882	0.302	0.98	
24-0ct	12:00	13:00	14.066	0.281	1.00	
24-0ct	13:00	14:00	15.149	0.350	0.99	
24-0ct	14:00	15:00	17.103	0.409	0.99	
24-0ct	15:00	16:00	18.827	0.486		BACKGROUND 15:40 - 15:51
24-0ct	16:00	17:00	12.913	0.352	0.99	
24-0ct	17:00	18:00	7.760	0.188	0.99	
24-0ct	18:00	19:00	6.808	0.282	0.98	
24-0ct	19:00	20:00	4.839	0.182	0.99	CALIBRATION 19:35 - 19:47
24-0ct	20:00	21:00	1.226	0.049	0.98	
24-0ct	21:00	22:00	0.663	0.161	0.67	
24-0ct	22:00	23:00	0.692	0.100	0.83	
24-0ct	23:00	24:00	0.909	0.060	0.96	
25-0ct	00:00	01:00	0.551	0.073	0.85	
25-0ct	01:00	02:00	0.694	0.095	0.84	
25-0ct	02:00	03:00	0.487	0.147	0.57	
25-0ct	03:00	04:00	0.317	0.126	0.47	
25-0ct	04:00	05:00	0.015	0.127	0.03	
25-0ct	05:00	06:00	0.037	0.162	0.05	
25-0ct	06:00	07:00	-0.060	0.177	-0.07	
25-0ct 25-0ct	07:00 08:00	08:00	0.440	0.170 0.212	0.48	
25-0ct 25-0ct	09:00	09:00 10:00	-0.007 0.308	0.336	-0.01	CALIBRATION 09:06 - 09:18
25-0ct	10:00	11:00	-0.066	0.690	-0.02	CALIBRATION 09:06 - 09:18
25-0ct	11:00	12:00	5.531	0.342	0.96	
25-0ct	12:00	13:00	10.269	0.437	0.98	
25-0ct	13:00	14:00	13.952	0.354	0.99	
25-0ct	14:00	15:00	20.371	0.679	0.99	
25-0ct	15:00	16:00	22.164	0.858	0.98	
25-0ct	16:00	17:00	18.134	0.496	0.99	
25-0ct	17:00	18:00	12.518	0.163	1.00	
25-0ct	18:00	19:00	5.995	0.137	0.99	t .
25-0ct	19:00	20:00	3.253	0.100	0.99	
25-0ct	20:00	21:00	2.139	0.111		CALIBRATION 20:35 - 20:43
25-0ct	21:00	22:00	0.565	0.114	0.73	20140
25-0ct	22:00	23:00	0.818	0.238	0.59	
25-0ct	23:00	24:00	0.451	0.106	0.67	

LOCATION: AZUSA SCAQMD AIR MONITORING STATION
INSTRUMENT: TDLAS
SPECIES: HN03 - 1 HOUR AVERAGES

PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE	START	END	MIXING	95%	CORR.	COMMENTS
DD-MMM-YY	TIME	TIME	RATIO	LIMIT	COEFF.	
##========	PDT	PDT	(PPBV)	(PPBV)		
26-Oct	00:00	01:00	0.205	0.171	0.26	
26-0ct	01:00	02:00	0.443	0.164	0.51	
26-0ct	02:00	03:00	0.758	0.131	0.79	
26-0ct	03:00	, 04:00	0.580	0.134	0.69	
26-0ct	04:00	05:00	0.416	0.122	0.60	
26-0ct	05:00	06:00	0.609	0.109	0.78	
26-0ct	06:00	07:00	0.373	0.068	0.77	
26-0ct	07:00	08:00	0.335	0.103	0.58	
26-0ct	08:00	09:00	0.263	0.206	0.27	CALIBRATION 08:23 - 08:42
26~0ct	09:00	10:00	0.890	0.130		CALIBRATION 08:59 - 09:09
26-0ct	10:00	11:00	8.211	0.343	0.98	
26-0ct	11:00	12:00	13.321	0.345	0.99	
26-0ct	12:00	13:00	12.799	0.224	1.00	BACKGROUND 12:47 - 13:00
26-0ct	13:00	14:00	9.465	0.409	0.98	
26-0ct	14:00	15:00	11.295	0.387	0.99	
26-0ct	15:00	16:00	10.529	0.247	0.99	
26-0ct	16:00	17:00	9.868	0.308	0.99	
26-0ct	17:00	18:00	10.397	0.292	0.99	
26-0ct	18:00	19:00	8.585	0.391	0.98	
26-0ct	19:00	20:00	8.031	0.340	0.98	
26-0ct	20:00	21:00	8.883	0.316		CALIBRATION 20:25 - 20:37
26-0ct	21:00	22:00	8.179	0.194	0.99	
26-0ct	22:00	23:00	3.583	0.192	0.97	
26-0ct 27-0ct	23:00	24:00	2.961	0.073	0.99	
27-0ct	00:00 01:00	01:00 02:00	4.523	0.242	0.97	
27-0ct	02:00	02:00	4.835 4.638	0.263 0.136	0.97 0.99	
27-0ct	03:00	04:00	3.954	0.130	0.99	
27-0ct	04:00	05:00	4.418	0.129	0.99	
27~0ct	05:00	06:00	4.845	0.183	0.99	
27~0ct	06:00	07:00	3.740	0.153	0.98	
27-0ct	07:00	08:00	2,488	0.190	0.94	
27-0ct	08:00	09:00	4,161	0.117	0.99	
27-0ct	09:00	10:00	3.474	0.290		CALIBRATION 09:27 - 09:39
27-0ct	10:00	11:00	3.419	0.085	0.99	00100
27-0ct	11:00	12:00	3.004	0.161	0.97	
27-0ct	12:00	13:00	3.625	0.085	0.99	
27-0ct	13:00	14:00	4.727	0.117	0.99	
27-0ct	14:00	15:00	7.442	0.218	0.99	
27-0ct	15:00	16:00	10.090	0.424	0.98	
27-0ct	16:00	17:00	5.502	0.223	0.98	
27-0ct	17:00	18:00	1.671	0.212	0.87	
27-0ct	18:00	19:00	0.951	0.088	0.92	
27-0ct	19:00	20:00	0.900	0.139	0.82	
27-0ct	20:00	21:00	1.062	0.110		CALIBRATION 20:34 - 20:45
27-0ct	21:00	22:00	1.503	0.054	0.99	
27-0ct	22:00	23:00	0.505	0.180	0.52	
27-0ct	23:00	24:00	0.655	0.080	0.88	

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS
SPECIES: HN03 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE DD-MMM-YY	START TIME PDT	END TIME PDT	MIXING RATIO (PPBV)	95% LIMIT (PPBV)	CORR.	COMMENTS
=========						
28-0ct	00:00	01:00	1.181	0.115	0.91	
28-0ct	01:00	02:00	0.938	0.187	0.74	
28-0ct	02:00	03:00	1.047	0.126	0.88	
28-0ct	03:00	04:00	0.678	0.213	0.57	
28-0ct	04:00	05:00	1.108	0.093	0.93	
28-0ct	05:00	06:00	1.137	0.169	0.83	
28-0ct	06:00	07:00	0.471	0.203	0.45	
28-0ct	07:00	08:00	0.337	0.083	0.67	
28-0ct	08:00	09:00	0.835	0.148	0.78	
28-0ct	09:00	10:00	0.221	0.078	0.53	CALIBRATION 09:31 - 09:43
28-0ct	10:00	11:00	3.138	0.080	0.99	
28-0ct	11:00	12:00	4.232	0.170	0.98	
28-0ct	12:00	13:00	5.563	0.133	0.99	
28-0ct	13:00	14:00	7.002	0.154	1.00	
28-0ct	14:00	15:00	8.424	0.172	1.00	
28-0ct	15:00	16:00	10.756	0.294	0.99	
28-0ct	16:00	17:00	8.831	0.250	0.99	
28-0ct	17:00	18:00	6.130	0.221	0.99	•
28-0ct	18:00	19:00	3.637	0.325	0.93	
28-0ct	19:00	20:00	1.965	0.076	0.98	
28-0ct	20:00	21:00	1.476	0.064	0.98	
28-0ct	21:00	22:00	1.608	0.141	0.93	CALIBRATION 21:38 - 21:52
28-Oct	22:00	23:00	1.690	0.051	0.99	
28-0ct	23:00	24:00	1.333	0.095	0.95	
29-0ct	00:00	01:00	1.257	0.060	0.98	
29-0ct	01:00	02:00	1.367	0.225	0.80	
29-0ct	02:00	03:00	0.787	0.126		
29-0ct	03:00	04:00	0.474	0.176	0.51	
29-0ct	04:00	05:00	0.106	0.115	0.20	
29-0ct	05:00	06:00	0.044	0.164	0.06	
29-0ct	06:00	07:00	0.219	0.096	0.45	
29-0ct	07:00	08:00	0.513	0.219	0.46	
29-0ct	08:00	09:00	0.554	0.076	0.85	
29-0ct	09:00	10:00	0.303	0.149		CALIBRATION 09:14 - 09:29
29-0ct	10:00	11:00	1.782	0.091	0.97	
29-0ct	11:00	12:00	3.507	0.092	0.99	
29-0ct	12:00	13:00	4.462	0.209	0.98	041 500 5 500 500 500 500 500 500 500 500
29-0ct	13:00	14:00	8.019	0.247		CALIBRATION 12:56 - 13:18
29-0ct	14:00	15:00	9.128	0.328	0.99	
29-0ct 29-0ct	15:00	16:00	8.595	0.232	0.99	
29-0ct	16:00 17:00	17:00	8.862	0.261	0.99	
		18:00	3.668	0.151	0.98	t
29-0ct 29-0ct	18:00 19:00	19:00	1.363	0.148	0.90	
29-0ct	20:00	20:00	1.018	0.076	0.95	
29-0ct	21:00	21:00 22:00	1.443	0.063	0.98	
29-0ct 29-0ct	22:00	23:00	0.827 0.966	0.265 0.242	0.57	CALIBRATION OF 15
29-0ct	23:00	24:00	1.277			CALIBRATION 22:15 - 22:26
29-001	23.00	£4:00	1.211	0.108	0.94	

STUDY NAME: LA ACID PRECIPITATION INTERCOMPARISON STUDY LOCATION: AZUSA SCAQMD AIR MONITORING STATION INSTRUMENT: TDLAS

SPECIES: HN03 - 1 HOUR AVERAGES
PERIOD: SEPTEMBER 30 - OCTOBER 30, 1993

DATE	START	END	MIXING	95%	CORR.	COMMENTS
DD-MMM-YY	TIME	TIME	RATIO	LIMIT	COEFF.	
	PDT	PDT	(PPBV)	(PPBV)		
===========	=======================================	=======				
30-0ct	00:00	01:00	2.192	0.204	0.92	
30-0ct	01:00	02:00	0.153	0.127	0.26	
30-0ct	02:00	03:00	0.344	0.126	0.52	
30-0ct	03:00	, 04:00	0.544	0.138	0.66	
30-0ct	04:00	05:00	0.840	0.165	0.75	
30-0ct	05:00	06:00	~0.065	0.160	-0.09	
30-0ct	06:00	07:00	0.833	0.095	0.89	
30-0ct	07:00	08:00	0.256	0.172	0.31	
30-0ct	08:00	09:00	-0.103	0.259	-0.09	CALIBRATION 08:29 - 08:40
30-0ct	09:00	10:00	0.748	0.314	0.46	
30-0ct	10:00	11:00	2.703	0.185	0.95	
30-0ct	11:00	12:00	7.109	0.320	0.98	CALIBRATION 10:57 - 11:18
30-0ct	12:00	13:00	6.410	0.305	0.98	
30-0ct	13:00	14:00	7.705	0.406	0.97	
30-0ct	14:00	15:00	8.287	0.392	0.98	
30-0ct	15:00	16:00	10.020	0.368	0.99	
30-0ct	16:00	17:00	8.672	0.462	0.97	
30-0ct	17:00	18:00	9.585	0.428	0.98	CALIBRATION 17:48 ~ 17:59
30-0ct	18:00	19:00	4.998	0.437	0.93	
30-0ct	19:00	20:00	6.126	0.441	0.95	
30-0ct	20:00	21:00	6.060	0.312	0.98	
30-0ct	21:00	22:00	6.256	0.604	0.92	
30-0ct	22:00	23:00	4.201	0.199	0.98	
30-0ct	23:00	24:00	4.153	0.255	0.97	END OF STUDY

## **NOTES**

## NOTES